

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
22 March 2001 (22.03.2001)


PCT

(10) International Publication Number  
**WO 01/19235 A1**

- (51) International Patent Classification<sup>7</sup>: **A61B 1/04**, 1/313, 1/002
- (21) International Application Number: PCT/US00/25107
- (22) International Filing Date:  
13 September 2000 (13.09.2000)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
60/153,568 13 September 1999 (13.09.1999) US  
60/156,478 28 September 1999 (28.09.1999) US  
60/187,305 6 March 2000 (06.03.2000) US  
09/518,954 6 March 2000 (06.03.2000) US  
60/212,935 20 June 2000 (20.06.2000) US
- (63) Related by continuation (CON) or continuation-in-part (CIP) to earlier application:  
US 09/518,954 (CIP)  
Filed on 6 March 2000 (06.03.2000)
- (71) Applicant (for all designated States except US): **VISION-SCOPE, INC.** [US/US]; 15 Fatima Drive, Ashland, MA 01721 (US).
- (72) Inventors; and  
(75) Inventors/Applicants (for US only): **REMIJAN, Paul** [US/US]; Blodgett Road, RR 3, Box 3719, Holland, MA 01521 (US). **LABOMBARD, Denis** [US/US]; 7 Boardman Street, Georgetown, MA 01833 (US).
- (74) Agents: **HOOVER, Thomas, O. et al.**; Hamilton, Brook, Smith & Reynolds, P.C., Two Militia Drive, Lexington, MA 02421 (US).
- (81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.
- (84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian

[Continued on next page]

(54) Title: **MINIATURE ENDOSCOPE SYSTEM**

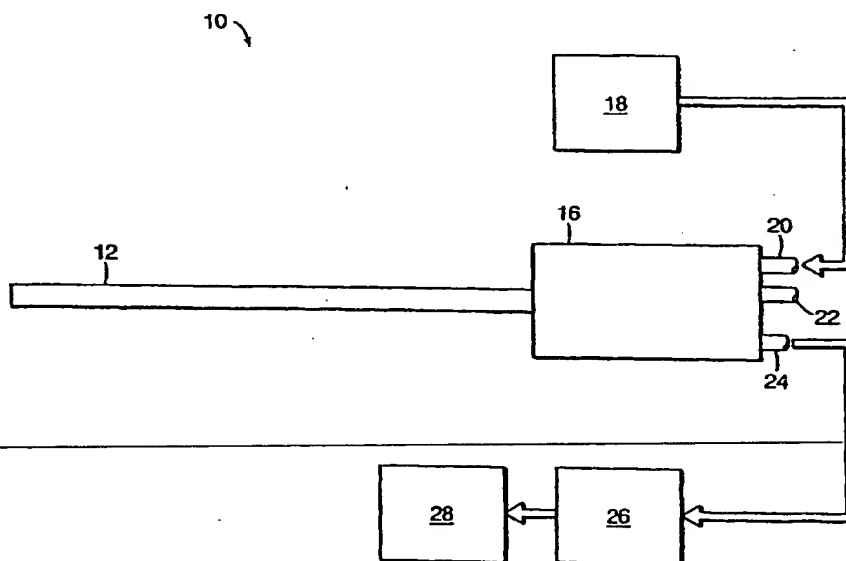

(57) Abstract: The present invention relates to a small diameter imaging probe or endoscope (10), a solid state imaging device (44), and a light transmitting path (40, 30, 42) that collects light at a distal end of the probe and directs the light along the length of the probe to the imaging device. The invention also relates to a small diameter endoscope having a light transmitting path with a light absorbing layer (32) and a super clad layer (68) defining the image aperture. The invention relates to a small diameter endoscope system for imaging of objects or tissue within a body. An image relay (42) is used to couple image light between optical elements of the probe such that an image is detected by an imaging sensor (44) at a proximal end of the device.

BEST AVAILABLE COPY

WO 01/19235 A1



patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

— Before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments.

**Published:**

— With international search report.

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

-1-

## MINIATURE ENDOSCOPE SYSTEM

## RELATED APPLICATION

This application claims the benefit of U.S. Provisional Application Nos. 60/212,935 filed June 20, 2000, 60/187,305 filed March 6, 2000, 60/156,478 filed September 28, 1999 and 60/153,568 filed September 13, 1999 and is a Continuation-in-Part (CIP) of 09/518,954, filed March 6, 2000, the teachings of which are incorporated herein by reference in their entirety. This application relates to U.S. Application No. 09/520,648 filed March 6, 2000, and U.S. Application No. 09/521,044, filed March 6, 2000, the contents of the above applications are incorporated herein by reference in their entirety.

## BACKGROUND OF THE INVENTION

Endoscopes are devices which allow visual examination inside a hollow cavity. In the field of medicine, the use of endoscopes permits inspection of organs for the purpose of diagnosis, viewing of a surgical site, sampling tissue, or facilitating the safe manipulation of other surgical instruments. Laparoscopes are used particularly for examining organs in the abdominal area. Laparoscopes typically include a light pipe for illuminating the region to be viewed, at least one lens assembly for focusing and relaying the image of the illuminated object, and a housing for the entire assembly which is structured to minimize tissue damage during the surgical procedure. The light pipe can include a fiber optic element for illuminating the site. The laparoscope housing includes a distal section that can be inserted within a body cavity and a proximal section which can include a handle that a user grips to position the distal end near the surgical site.

Existing laparoscopes can include an imaging device such as a charge coupled device (CCD). This device can capture an image of an object being viewed and convey it to a display device, such as monitor. There is a continuing need to improve on the operational features and manufacturability of endoscope systems that improve imaging capability and reduce the risk to the patient.

## SUMMARY OF THE INVENTION

The present invention relates to a small diameter imaging probe or endoscope having improved resolution and field of view. The distal end of the probe, that is inserted into the tissue under examination, is preferably less than 2mm  
5 in diameter to reduce trauma at the point of insertion and thereby provide access to sites that are otherwise unavailable for endoscopic examination.

In a preferred embodiment, the endoscope has an optical waveguide or elongated rod, which can be made of a transparent material such as a high refractive index glass, an illumination channel, an optical system and an imaging sensor. The  
10 outer diameter of the elongated rod is preferably in the range of 0.6 - 1.6 mm. The imaging device is optically coupled to the rod using one or more lenses.

The waveguide can be used to conduct light from a distal end to a proximal end of the device. The rod can have an outer surface which is coated with an absorbing material or light absorbing layer to inhibit internal reflection and  
15 scattering of light. One or more lenses at the distal end of the rod can provide enhanced coupling of light into the distal aperture of the rod.

The illumination channel can surround the rod and transmits light from a light source to an object being examined. The illumination channel is formed with or on the outer surface of the light absorbing layer. A dispersive element can be  
20 placed at the distal end of the illumination channel to enhance illumination of the region of interest.

The imaging device can be a charge coupled device (CCD), a CMOS imaging device or other solid state imaging sensor having a two dimensional array of pixel elements. The sensor can capture an image as an object being viewed and  
25 transmit it to a computer for storage, processing and/or a display.

In another preferred embodiment, the endoscope has an optical system which includes distal optics and an image relay or tube. The tube can have an inner channel such as a hollow cylinder coated with a light absorbing material to inhibit internal reflection and scattering of light. The endoscope has a duplex configuration  
30 which uses a beamsplitter to direct illumination light along the same optical path or air tube used for the transfer of image light from an object being imaged.

The system can use a sheath assembly to provide a sterile barrier over the handle. The barrier can be disposable along with the needle probe.

The light source can be a high power light source. The light can be concentrated by source optics to a polarizer and to a beam splitter before traveling  
5 through the tube. The illumination light can be polarized to improve delivery and collection efficiency.

The miniature endoscope system can be used for orthopedic, rheumatologic, general laparoscopic, gynecological or ear, nose and throat procedures, for example. Although many applications require a small diameter to reduce trauma, certain  
10 applications can accommodate larger diameters.

The foregoing and other objects, features and advantages of the invention will be apparent from the following more particular description of preferred embodiments of the invention, as illustrated in the accompanying drawings in which like reference characters refer to the same parts throughout the different views. The  
15 drawings are not necessarily to scale, emphasis instead being placed upon illustrating the principles of the invention.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates a schematic illustration of a preferred embodiment of the endoscope;

20 FIG. 2 shows a cross-sectional view of the endoscope optical system;

FIG. 3 illustrates a front view of an embodiment of the endoscope optical system;

FIG. 4 shows a schematic illustration of an alternate embodiment of the endoscope shown in FIG. 1;

25 FIG. 5 illustrates rectangular optics and a rectangular image transmission rod of an endoscope transmitting light to an imaging device;

FIG. 6 illustrates a super-clad structure integrated over a square or  
rectangular transmission path of an endoscope;

FIG. 7 illustrates a perspective view of a preferred embodiment of the  
30 invention;

FIG. 8 illustrates an endoscope having an air tube and a duplex configuration;

FIGS. 9 and 10 show a side view and a perspective view, respectively, of a miniature endoscope;

5        FIG. 11 illustrates a rod tip of a miniature endoscope;

FIG. 12 shows a cross-sectional view of a miniature endoscope;

FIG. 13 shows a detailed view of the light transfer and imaging system of the endoscope of FIG. 12;

FIG. 14 illustrates a rod tip of an endoscope mounted within a needle;

10       FIG. 15 shows a cross-sectional view of an alternate embodiment of an endoscope;

FIG. 16 shows a detailed view of the light transfer and imaging system of the endoscope of FIG. 15;

FIG. 17 shows a micro endoscope with an external light source;

15       FIG. 18 illustrates an alternate configuration of a lighting system for a miniature endoscope;

FIG. 19 illustrates a cannula for a miniature endoscope; the cannula having an illumination cannula;

FIG. 20 shows a cannula having a stylet;

20       FIG. 21 is a perspective view of an alternative embodiment of the miniature endoscope;

FIG. 22 is a top sectional view of the miniature endoscope;

FIG. 23 is a side view, a portion shown in hemline of the miniature endoscope;

25       FIG. 24 is a rear view of the miniature endoscope;

FIG. 25A is a front view of the base of the miniature endoscope with the needle not attached;

FIG. 25B is an enlarged view of a portion of the connection of the endoscope of FIG. 25A;

30       FIG. 26 is a side sectional view of the miniature endoscope;

FIG. 27A is an enlarged sectional view of a portion of the endoscope of FIG. 26;

FIG. 27B is an enlarged sectional view of the distal end of the endoscope of FIG. 26;

FIG. 28 is a sectional view of the miniature endoscope taken along the line 28-28 of FIG. 26;

5 FIG. 29A is an enlarged sectional view of a portion of the endoscope of FIG. 28;

FIG. 29B is an enlarged sectional view of a portion of the endoscope of FIG. 28.

#### DETAILED DESCRIPTION OF THE INVENTION

10 A preferred embodiment of the invention is illustrated in FIG. 1 which shows a miniature endoscope 10. The endoscope 10 has an image transmission path such as an optical waveguide or elongated rod 12 used to view objects to be examined. The elongated rod 12 can be attached to a handle 16. The handle 16 can house a light source input 20 which can connect to a light source 18. In a preferred  
15 embodiment, the light source input 20 such as a fiber optic cable optically couples the light source 18 to an illumination channel within the endoscope 10. The handle 16 can also house a power input 22, used to provide power to the endoscope 10. Alternatively, the light source and/or power source can be mounted within the handle.

20 The handle 16 can also house an image output 24. The image output 24 provides a connection between an imaging device in the endoscope and an electronic storage and/or display device. In one embodiment, the storage device is a computer 26 which is connected to a monitor 28. The imaging device can be a charge coupled device or other pixellated flat panel sensor.

25 FIG. 2 shows a cross-sectional view of an embodiment of the microendoscope 10. The elongated rod 12 can have a transparent material such as a high index glass rod 30 having a refractive index greater than one, an illumination channel 34, an optical element or distal optics 38 and proximal optics 42.

The distal optics 38 can form a virtual image of an object being examined.  
30 In a preferred embodiment, the distal optics 38 can be one or more plastic lenses. The high index glass rod or core 30 links the distal optics 38 to relay optics 42

located in a proximal end of the endoscope 10. In one embodiment, the distal-optics comprise two lenses. The high index glass core 30 can have a refractive index of 1.85 and can reduce the optical path between a virtual image created by the distal optics 38 and the relay optics 42. The high index glass rod 30 is preferably free of  
5 birefringence to produce an aberration free image at an image sensor 44. Stress within the glass core 30 is necessary for mechanical strength. In a preferred embodiment, the glass core 30 is made of SF57, a pochels glass, which is a glass that can be mechanically stressed without introducing stress birefringence.

The high index glass core 30 can have a tunnel barrier or light absorbing  
10 layer or sheath 32. The purpose of the tunnel barrier or sheath 32 is to absorb unwanted light. One option for a tunnel barrier is described in U.S. Patent No. 5,423,312, the entirety of which is incorporated herein by reference. This option employs a glass rod having an outer surface that has been roughened and blackened to provide an absorbing barrier. In contrast, the present invention leaves the glass  
15 rod intact and provides an external coating having a lower index of refraction to absorb light crossing the rod's external surface. In a preferred embodiment, the tunnel barrier or absorbing sheath 32 is EMA or extramural absorption glass (available from Shott Fiber Optics, Southbridge, MA). The EMA glass can be extruded during a fiber optics drawing process. The extrusion process leaves the  
20 outer surface of the high index glass rod intact. The extruding process instead adds material to the outer surface of the high index glass rod 30 to create a reflective boundary. The extruding process can be performed using a bar in tube drawing process. Similarly, the extruding process can be performed using a differential bar in tube drawing process. In a preferred embodiment, the EMA glass is  
25 approximately 5-10  $\mu\text{m}$  thick. The EMA glass can have a refractive index of 1.6, for example.

The illumination channel 34 can be used to provide light from a light source to an object being illuminated. In one embodiment the illumination channel is coupled to glass fiber which is coupled to a light source. In a preferred embodiment,  
30 the illumination channel 34 can be extruded during a fiber optics drawing process. In another embodiment, this fiber optic drawing process can be performed in a



second drawing process. The illumination channel can have a wall thickness of 0.15mm and can have a refractive index of 1.5 for example.

The image channel or illumination channel 34 can have an outer sheath 36. In a preferred embodiment, the outer sheath 36 is a polyamide coating. The coating can be between 100 and 150  $\mu\text{m}$  thick. The polyamide coating can be applied in a final fiber optics drawing process. Alternatively, one or more of the layers on the rod can be applied by a coating, dipping or deposition process. The polyamide coating can provide strength to the glass core 30. If a glass shatter event were to occur, the polyamide coating can contain the glass from the core 30 to prevent injury to the patient. An outer metal or plastic tube can also be used to enclose the distal end of the device.

The elongated rod 12 can also have a binary phase ring 40 located at its distal end. The ring 40 is positioned on the elongated rod 12 so as to abut the illumination channel 40. The binary phase ring is coupled to the illumination channel in one embodiment. The binary phase ring 40 disperses light traveling through the illumination channel 34 to provide even illumination of the field of view. In a preferred embodiment, the binary phase ring 40 is made from a plastic material. The binary phase ring 40 can also have a distal window 46. The window can be mounted flush against the distal optics 38.

The elongated rod 12 of the endoscope 10 in one embodiment has an outer diameter under 2mm. In another embodiment, the endoscope 10 has an outer diameter of 1.6 mm or less. In a preferred embodiment requiring a small entry site, the endoscope 10 has an outer diameter of 1 to 1.2 mm.

FIG. 3 illustrates a front view of an embodiment of an endoscope 10. The endoscope 10 can have an image light channel 58 and a super-clad structure 68. The image light channel 58 can include a light absorbing layer 56. The super-clad structure 68 can include a first coating or layer 64, a second coating or layer 66 and an illumination channel 62. The super-clad structure 68 directs light through the endoscope 10.

The image light channel 58 can be made from a transparent material or high index glass core 52. In a preferred embodiment, the core 52 is made from a material having a constant refractive index to eliminate deviation of light passing through the

material. The constant refractive index may be achieved after the stress of a fiber drawing process by using a pockels glass core, for example. Pockels glasses exhibit zero birefringence when placed in compression or tension. The constant refractive index may also be achieved by annealing the image light channel 58 after the fiber drawing process. The core 52 can also have a first diameter 54. In a preferred embodiment, the first diameter 54 is 1.20 mm.

The light absorbing layer 56 of the image light channel 58, in a preferred embodiment, is a light absorbing glass. The light absorbing layer 56 can have a higher index of refraction than the core 52 and can be made from the same material as the core 52. Light absorbing colorants can be added to the light absorbing glass material to raise its index of refraction and increase its light absorption. In a preferred embodiment, the index of refraction of the light absorbing layer 56 is slightly higher than the index of refraction of the core 52. The light absorbing layer 56 can be applied to the core 52 using a fiber drawing process, for example.

The high index glass core 52 and light absorbing layer 56 can be formed from various types of glass materials. In one embodiment, the image light channel 58 can be formed from an F2 glass core and a BG-4 glass light absorbing layer. The F2 glass core can have a refractive index of 1.620. The BG-4 glass light absorbing layer can have a refractive index of approximately 1.65. In another embodiment, the image light channel 58 can be formed from an F7 glass core and a BG-2 glass light absorbing layer. The F7 glass core can have a refractive index of 1.625. The BG-2 glass light absorbing layer can have a refractive index of approximately 1.66.

The light absorbing layer 56 can have a thickness as low as 5  $\mu\text{m}$ . Preferably, the thickness of the light absorbing layer 56 is no greater than 10  $\mu\text{m}$ . The image light channel 58, formed of the core 52 and the light absorbing layer 56, can have a second diameter 60. In one embodiment, the second diameter 60 is 1.24 mm.

The illumination channel 62 has the first coating 64 and the second coating 66 to form a super-clad structure 68. The first coating 64 is located on an inner surface of the channel 62. The second coating 66 is located on an outer surface of the channel 62. The illumination channel 62 can be made from a high index of refraction material. In one embodiment, the illumination channel 62 can be made

from LG1 glass which can have a refractive index of approximately 1.82. Both the first coating 64 and the second coating 66 can be made from a low index of refraction material. In one embodiment, the coatings 64, 66 can be made from EG1 glass which can have a refractive index of approximately 1.50. In another  
5 embodiment, the coatings can be made from EG9 glass which can have a refractive index of approximately 1.56. The low index material can provide for illumination containment of the illumination channel 62. The illumination channel 62 can have a thickness of 30  $\mu\text{m}$ . The first 64 and second 66 coating layers can each have a thickness as low as 5  $\mu\text{m}$ , respectively. Preferably, the thickness of each of the first  
10 64 and second 66 coating layers is 10  $\mu\text{m}$ .

The super-clad structure 68 can be made by different processes such as a triple-glass, a tube-extrusion process, a dip coating process or chemical deposition combined with fiber drawing processes, for example.

In one embodiment of a process to fabricate a super-clad structure 68, the  
15 image light channel 58 can be exposed to a triple-glass tube-extrusion process, which can form the super-clad structure 68. A bar-in-tube fiber draw can then be used to fuse the super-clad structure 68 around the image light channel 58.

In another embodiment of forming a super-clad structure 68, an image light channel 58 can be dipped in a low index, high temperature polymer to form a first  
20 coating 64. A high index plastic can then be extruded over the polymer clad image light channel 58, to form an illumination channel 62. The entire structure can then be dipped in a low index polymer to form the second coating 66.

In another embodiment of a process of fabricating a super-clad structure 68, a metal layer can be chemically deposited onto both sides of an illumination channel  
25 62 to form a super-clad structure 68. In a preferred embodiment, the metal is aluminum. The super-clad structure 68 can then be fused to an image light channel 58 using a bar-in-tube fiber drawing process. The super-clad structure 68 and the image light channel 58, the endoscope 50 can have a third diameter 70. In one  
embodiment, the third diameter 70 is 1.65mm.

30 In an alternate embodiment, the endoscope can have an angled distal tip in the shape of a needle shown in FIG. 4. This tip provides for ease of insertion at the site to be examined.

The endoscope can also have square or rectangularly shaped distal optics which can form a virtual image of an object being examined. The endoscope can also have an image transmission path or image channel, such as an elongated rod, which can have a square or rectangularly shaped cross section. Similarly, the  
5 endoscope can have square or rectangularly shaped relay optics. By using rectangular optics or a rectangular transmission path, a more efficient transfer of light can be made from an object being viewed to an imaging device, which has a square or rectangular imaging area. All light from an object being imaged can be directly transferred to the imaging area, with little to no light wasted during the  
10 transfer.

Generally, endoscopes have circular optics which can transmit light rays to a rectangularly shaped imaging device. For endoscopes having optics with circular cross-sectional areas greater than the cross-sectional area of the imaging device, a portion of the light rays traveling in the arcuate areas of the circular optics will not  
15 be transmitted to the imaging device. These light rays can be considered as "wasted" since the light rays fail to intersect the imaging device and are, therefore, unused.

FIG. 5 illustrates rectangular distal optics or optical elements 88 for an endoscope which can transmit light rays to an imaging device 44. In this  
20 embodiment, all light rays from the rectangular distal optics 88 can be transferred to the imaging device 84. More light from the object being imaged can therefore be transferred to the imaging device 84 with little waste. A rectangularly shaped transmission path 90 can be used to transfer the light from the distal optics 88 to the imaging device 44. Rectangularly shaped relay optics 86 can also be used to transfer  
25 the light from the distal optics 88 to the imaging device 44.

When a square or rectangular transmission path is used in a microendoscope, the inner surface of a super-clad layer of the microendoscope can be shaped to conform to the outer surface of the transmission path. FIG. 6 illustrates a  
microendoscope 94 having a rectangular light transmission path 96 and a super-clad  
30 layer 98. The light transmission path 96 has an outer surface 100 which can be coated with a light absorbing layer which conforms to the geometry of the outer surface 100. When the super-clad layer 98 is to be applied to or extruded over the

light transmission path 96, an inner surface 102 of the super-clad layer 98 can conform to the geometry of the light transmission path 96, as illustrated. For a square light transmission path 96, the inner surface 102 of the super-clad layer 98 can be extruded square over the transmission path 96.

5           FIG. 7 shows a perspective view of a miniature needle endoscope in accordance with the invention. Fiber and electrical cables are connected to the proximal end of handle 16 or needle 12 for insertion into a patient is attached at a distal end of handle 16.

A preferred embodiment of the invention can be considered as three  
10 subassemblies. A first subassembly shown in FIG. 9 is the outer handle housing 120 having a distal rod connector 122. A second subassembly is the inner handle 140 shown in FIG. 12. Inner handle 140 includes proximally located fiber and electrical connectors 142 and 144 that are attached to an inner cage assembly 146. The fiber connector 142 connects light from an external source to an illumination annulus 154  
15 which couples light to an illumination channel 308 in needle 240 as shown in FIG. 19. Light collected through needle 240 is coupled to lenses 150 and 152 onto an imaging sensor such as CCD 148.

FIGS. 9 and 12-14 illustrate a disposable third assembly having a rod and needle with a distal lens assembly 162 that is attached to a sterile sleeve assembly  
20 160. The sleeve assembly 160 includes a sleeve 164 that extends over the handle or base unit 202. The distal end of sleeve 164 is secured between plastic frames 166, 170 which can form a mounting hub 218. Frame 166 has a hole 168 that connects to rod and lens assembly 162. Frame 170 connects to rod connector or interface connector 122.

25           FIG. 8 illustrates an endoscope, identified generally as 130. The endoscope 130 can have an optical system 123 and a handle 124. The optical system 123 can include a tube 103 having a distal end 112, a proximal end 111 and distal optics 117 and can have an outer diameter between 0.6 and 2.0 mm with a preferred outer  
diameter of about 1.6 mm. The optical system 123 can be disposable. The handle  
30 portion 124 can include proximal optics 105, an image polarizer 106, an image sensor 107 and a beam splitter 104. The proximal optics 105 can include an achromatic lens. The beam splitter 104 can be coated with a dielectric coating. The

beam splitter coating can be designed to provide maximum reflection of "s polarized" illumination flux and maximum transmission of "p polarized" image light. The curvature of the distal optics 117 can be chosen to minimize retro-reflections of illumination flux appearing in the image.

5           The endoscope 130 can have a duplex configuration wherein the duplex configuration integrates illumination optics and uses the beam splitter 104 to direct illumination energy along the same optical path used for image light transfer. "Duplex" refers to the optical components and optical path used by illumination flux and image light.

10           The basic optical components used for both the image light and illumination flux in the endoscope 130 are shown in FIG. 8. As part of the imaging component of the endoscope 130, an object plane 101 can be located from 2 to 20 mm in front of a distal tip 126 of the endoscope 130. The distal optics 117 form a demagnified virtual image 114, located just outside the distal tip 126. A narrow beam of image  
15 light from the virtual image 114 can pass through the tube 103, through a dielectric coated beam splitter 104, toward proximal optics 105, and eventually to an image sensor 107, where a real image is formed. Image polarizer 106 can be a linear polarizer that is "crossed" with an illumination polarizer 108 to block retro-reflected illumination flux originating from surfaces of the distal optics.

20           The tube 103 can be a stainless steel extrusion having a rough inner surface which can be coated with a light absorbing coating, such as spray paint. For example, Krylon #1602, a dull black paint can be used. The tube 103 can have an inner diameter of 1.5 mm with the light absorbing inner wall to reduce or eliminate veiling or scattered light at the image sensor 107. The tube 103 can be filled with air  
25 or some other inert gas, or can be evacuated.

          The image channel or image relay 103 functions to minimize or absorb unwanted light and hard to image light to prevent veiling glare. The image relay 103 provides high resolution of the optical image, 114 at the plane of the imaging device, removes intermediate image planes and reduces the tolerances needed for  
30 optical alignment and optical fabrication. The image relay 103 has an inner tunnel wall that can absorb light diverging from the optics 117. The rough wall surface can disperse up to about 95% or more of unwanted light. The image relay 103 can have

-13-

a length to diameter (L to D) ratio of between 40:1 and 60:1. The length of the tunnel can be approximately 60 mm. The length of the image relay 103 affects proper illumination of an imaging device, helps control depth of field of view, increases F number for adequate depth of field of view. The image relay 103 can  
5 also be disposable.

The optical element or distal optics 117 on the tube 103 can be a polymer lens or an epoxy lens. The distal optics can have a diameter of 1.5 mm. The distal optics 117 can be a single distal lens to reduce retro-reflections. The distal optics 117 can be formed from an epoxy using an injection method. In this method a  
10 mandrel can first be placed within the tube 103 from the distal end 112 to the proximal end 111. Epoxy can then be ejected from the needle within 1 mm of the distal end 112 of the tube 103. The epoxy can then be exposed to ultraviolet (UV) light to cure the epoxy. The distal optics 117 can be formed as a concave/negative lens because of the capillary action caused by the air tube 103 after ejection of the  
15 epoxy from the needle. The distal 117 and proximal 105 optics can allow control of the size of an image.

The area surrounding the proximal end 111 of the tube can be carefully sculpted and blackened to reduce retro-reflected energy at the image sensor 107 originating from the illumination flux overfill of the air tube 103. The proximal  
20 optics 105 are "looking at" this overfill area and the image polarizer 106 can transmit scattered, unpolarized light to the image sensor 107.

The endoscope 130 can be linked via beamsplitter 104 to an illumination system 116. The illumination system 116 can include an illumination source 110 such as a COTS lens end Halogen Lamp having a 0.25 inch diameter from Gilway  
25 Technical Lamp. The COTS "Lens End" lamp can have high flux output from a small filament. The illumination source 110 can provide high color temperature visible light for object plane 101 illumination. Source optics 109 can concentrate illumination flux at the proximal end 111 of the tube 103 and provide a low  
divergence beam to maximize transmission of illumination flux through the tube  
30 103. A beam splitter 104 can redirect illumination flux along an image light axis 115. Illumination polarizer 108 is a linear polarizer oriented to provide "s polarization" at the beam splitter to maximize reflection of illumination flux from

dielectric coated beam splitter 104, along axis 115. A light absorbing mechanism or beam dump 113 can remove unused portion of illumination flux from the system to reduce veiling background light that can find its way onto the image sensor.

5 Illumination optics must be carefully designed to maximize illumination at object plane. The illumination optics create a small spot of light at proximal end of air tube and a collimated beam for maximum transmission through air tube.

Illumination and image polarizers must provide high polarization purity with minimum absorption. For example, dichroic sheet polarizers can be inexpensive, but lossy. Calcite polarizers can be more efficient, but expensive and more  
10 difficult to accommodate in a simple optical design.

Unused illumination flux transmitted by the beam splitter must be completely removed from the system because the proximal optics are "looking at" the dump area 113. The image polarizer will transmit scattered, unpolarized light to the image sensor.

15 All retro-reflections can be minimized using well known "optical isolation" configurations, but not totally eliminated. Therefore, electronic image processing may be required to produce an acceptable image. Since the retro-reflection pattern at the image sensor is unique for each scope, this unwanted light distribution can be recorded for each scope, stored in an image buffer, and subtracted from the video  
20 image in real time.

The endoscope 130 can be inserted into a body using a cannula. During an insertion procedure, a cannula can first be inserted into a site within a body. The optical system 123 of the endoscope 130 can then be inserted within the cannula which can have an outer diameter of 1.6 mm. The optical system 123 can pass  
25 through the cannula and into the body to provide the user with an image of the site.

The system can be used with a disposable sleeve or sheath to aid in maintaining a sterile environment and reduce the sterilization requirements prior to reuse.

FIGS. 9 and 10 illustrate a miniature endoscope, given generally as 200, in  
30 both a side and a perspective view respectively. The endoscope 200 can include a base unit 202 and a sheath assembly 160. The base unit can include a cable 224 which can provide power to an internal light source within the base unit 202. The



sheath assembly can include a sterile barrier 164 and a probe or rod and lens assembly 162. The rod and lens assembly 162 can be formed of a rod or waveguide 204 and a object lenses 206. The waveguide can be a hollow channel. The probe can have an annular illumination channel around the waveguide. The probe can have a length between 2 cm and 10 cm. The sterile barrier 164 and the rod and lens assembly 162 can be attached to a mounting hub 218 or second locking element which secures to a first locking element of the base unit 202 of the endoscope 200. The hub 218 can include an interface connection 122 or first locking element that allows the sheath assembly 160 to attach to the base unit 202. The interface connection 122 can be a securing mechanism such as a locking mechanism. The sterile barrier 164 can attach to the mounting hub 218 by bonding. The bonding can include cementing between the sterile barrier 164 and the hub 218, for example. The mounting hub 218 can include a locking mechanism 216 such as a luer lock for example. The locking mechanism 216 can allow connection between the miniature endoscope 200 and a needle such as a 14 gage cannula, for example (manufactured by Popper).

The rod and lens assembly 162 can include a rod tip 226 illustrated in FIG. 11. The rod tip 226 can have object lenses 206. These object lenses can include a first object lens 208 and a second object lens 210. The rod 204 of the rod and lens assembly 162 can be covered by a tube 214 or light absorbing boundary. The tube can be a dark coating in order to reduce or eliminate veiling or scattered light within the rod 204.

The sterile barrier 164 of the sheath assembly 160 can cover the entire base unit 202. This covering provides a sterility of the base unit 202 during a surgical procedure.

The miniature endoscope 200 can be inserted into a cannula or needle 240 as illustrated in FIGS. 12-16. Preferably the needle 240 has a blunt end. The needle can be a 14 gauge needle. To use the miniature endoscope 200 with the needle 240 in a surgical procedure, a sheath assembly 160 can first be placed on a base unit 202. The rod and lens assembly 162 of the sheath assembly 160 can lock into the interface connection 122 of the base unit 202. A needle or cannula 240, having a stylet 320, such as seen in FIG. 20, slidably mounted within the cannula, can be

inserted into a surgical site. In the case where a blunt needle or cannula 240 is used, the stylet 320 can cut into the tissue of a surgical site and thereby allow the needle 240 to be inserted into the surgical site. The stylet 320 can then be removed from the cannula 240. The stylet or obturator 320 fills the center portion of the cannula during insertion into a surgical site. The use of the stylet prevents coring of tissue, whereby a cylindrical portion of tissue enters the needle or cannula 240 and can clog the needle cavity. By having a stylet within the needle 240, no such tissue can enter the cannula 240 and can clog the needle cavity.

Once the stylet has been removed from the needle 240, the user can flush the surgical site with saline. Next, the rod and lens assembly 162 of the miniature endoscope 200 can be introduced into the needle 240. The rod portion 204 can be inserted within the needle 240 so that a user can obtain a view of the surgical site. The needle can include a locking mechanism on its proximal end, such as a luer lock for example. The luer lock can attach to the locking mechanism 216 of the mounting hub 218 thereby providing a secure attachment between the endoscope 200 and the needle 240.

FIGS. 12, 13 and 14 illustrate a cross sectional view of the miniature endoscope 200. The endoscope 200 can include a lighting system or light source 236 and an imaging system 238. The lighting system 236 can include a lamp 242, a polarizer 244 and a lens expander 246. The lamp 242 can be mounted within the base unit 202 by a light source housing 270 and can be a high output light source. The polarizer 244 can polarize light from the light source and direct light towards the expander 246. The lens expander 246 can direct light towards a prism 264.

The imaging system 238 of the endoscope 200 can include a first image path lens 150, a second image path lens 152 and a sheet polarizer 252. The imaging system can be mounted within a housing 140. The sheet polarizer 252 can help to eliminate back reflections from the rod and lens assembly 162. The polarizer 252 can have a polarization purity of  $10^{-3}$ .

FIG. 13 illustrates a light transfer and imaging system 262 of the endoscope 200 of FIG. 12. The light transfer and imaging system 262 can include a beamsplitter 264 which can be mounted within a housing 266 in the endoscope 200. The beamsplitter 264 can be a prism for example. The beamsplitter 266 can direct

light from the lens expander 246 into the rod 204 of the rod and lens assembly 162. This light can be directed at an object to be imaged. The beamsplitter 264 can also receive image light through the rod or channel 204 of an object being imaged and transfer that light to the polarizer 252 of the imaging system 238. The beamsplitter 5 264 can be mounted within the endoscope 200 at a Brewster's angle with such a mounting. The beamsplitter 264 in this example can form a  $33.5^\circ$  angle with respect to the long axis 272 of the rod. The beamsplitter 264 can also form a  $33.5^\circ$  angle with respect to the central axis of the imaging system 238.

FIG. 12 also illustrates an image sensor 148 mounted within the base unit 10 202 of the endoscope 200. The image sensor 148 can be mounted within an image sensor housing 258 within the endoscope 200. The image sensor 148 can be attached to an electrical cable connector 254 whereby the cable connector 254 can attach to a cable 230 to provide image signal data from an object being imaged to an external unit. The external unit can be a television screen, for example. The image 15 sensor 148 can be a charge coupled device (CCD). The CCD can be a 1/8 inch CCD. By using a 1/8 inch CCD, the user can quadruple the amount of light he receives from an image. When using a 1/8 inch CCD chip, the focal length of the endoscope 200 can be between 25 and 30 mm. Preferably the focal length is 27 mm.

FIG. 14 illustrates the rod tip 260 of the miniature endoscope 200 whereby 20 the rod tip 260 includes the first object lens 208, the second object lens 210 and a dark coating or tube 214 around a rod 204. As shown, the rod tip 260 is mounted within a needle or cannula 240. Such insertion of the rod tip 260 within the cannula 240 can be done after the cannula 240 is inserted into a surgical site of interest. Once the rod tip 260 is placed in the cannula 240, the cannula 240 can lock on to the 25 base unit 202 by means of a locking mechanism.

FIGS. 15 and 16 illustrate an alternate to the imaging system 238 illustrated in FIGS. 12, 13 and 14. The imaging system 238 can include a first image path lens 150, a second image path lens 152 and a polarizer 280. The cross polarizer 280 can 30 be made from calcite and can eliminate back reflections created by the rod and lens assembly 162. The polarization purity of the cross polarizer can be between  $10^{-5}$  and  $10^{-6}$ . The cross polarizer 280 can increase light throughput by 15% to 20%. The polarizer 280 can include a first prism 282 and a second prism 284. The polarizer

280 can be attached to the housing 140 of the endoscope 200 by a polarizer housing 286.

FIG. 16 illustrates the light transfer and imaging system 262 of FIG. 15. Light directed from the lens expander 246 can be sent through the beamsplitter 264 and into the rod 204 to an object being imaged. Light from the object being imaged can be transferred back through the rod 204 and through the prism 264 into the beamsplitter 280. The beamsplitter can transfer the image light to the polarizer 280 which can eliminate back reflections created by the object lenses 206.

FIG. 17 illustrates a miniature endoscope 200 where the light source of the endoscope 200 is an external light source 290. The external light source can include a lamp 292 and light source optics 294. The lamp 292 can be a xenon lamp which can be 300 watts, for example. The optics 294 and lamp 292 of the external light source 290 can be coupled to the miniature endoscope 200 by a silica cable 296. The endoscope 200 can include a reducer 298 mounted within the base unit 202. The reducer 298 can reduce the cross sectional area of the source by a factor of 2-5 times. Preferably the reducer reduces by a factor of 3.5. When used with a xenon source, the reducer 298 can reduce the aperture size of source for efficient coupling into the probe waveguide. The use of a reducer 298 within the endoscope 200 can simplify the optics within the lighting system 236.

FIG. 18 shows a configuration of the endoscope 200 wherein the lighting system 236 is mounted within the base unit 202 parallel to the imaging system 238. With such a configuration, the lighting system 236 can include a mirror 302. The mirror 302 can be a fold mirror for example. The mirror 302 can be mounted within the endoscope 200 such that light from a light source 242 which travels through a polarizer 244 and an expander 246 can reflect from the mirror to travel to the prism 264.

FIG. 19 illustrates the cross section of a needle 240 wherein the needle acts a reducer to provide light to an object being imaged. The needle 240 can include an aperture 304. The aperture can be surrounded by a first cladding layer 306, an illumination channel 308 and a second cladding layer 310. The first cladding layer can have a first cladding layer thickness 312. The illumination channel 308 can include a channel thickness 314 which can be 10 microns. The second cladding

layer 310 can include a second cladding thickness 316 whereby the thickness can be 3 microns.

FIG. 20 illustrates a cannula 240 having a stylet. Prior to inserting a needle 240 into a surgical site, a stylet or obturator can be inserted within the needle 240.

5 The stylet can include a cutting surface 322 and a cleaning edge 324. When the stylet 320 and needle 240 are inserted into a surgical site, tissue can accumulate in an area between the stylet 320 and the needle 240. In order to eliminate this material from the area, the stylet 320 can include a cleaning edge 324 whereby the cleaning edge is formed of a less stiff material than is the cutting edge 322. When the stylet  
10 320 is pulled towards the user after insertion of the needle 240 in the surgical site, the weaker edge or the cleaning edge 324 will bend about the needle thereby cleaning or wiping away any tissue debris from the needle area. Such a cleaning function allows proper insertion of the microendoscope within the cannula and proper viewing of a surgical site.

15 FIG. 21 shows a miniature endoscope 400 in side perspective view. The endoscope 400 includes a base unit 402 and a sheath assembly 404. The base unit 402 includes an electrical connection 406 for the imaging device, such as a CCD and a fiber optic light source connection 408.

The sheath assembly 404 includes a sterile barrier 410 and a rod and lens  
20 assembly 412. The sterile barrier 410 and the rod and lens assembly 412 are attached to a mounting hub 414, which is secured to the base unit 402 of the endoscope 400. The mounting hub 414 is a light sheath hub with luer lockside port.

The hub 414 can include an interface connection 416 that allows the sheath  
25 assembly 404 to attach to the base unit 402. The interface connection 416 can be a securing mechanism such as a locking mechanism. The sterile barrier 410, as seen in FIG. 22, is attached to the mounting hub 414 by bonding. The bonding can include cementing between the sterile barrier 410 and the hub 414, for example.

~~The mounting hub 414 can include a locking mechanism 418 such as a luer~~  
lock or fitting for example. The locking mechanism 418 can allow connection  
30 between the miniature endoscope 400 and a needle such as a 14 gage cannula, for example (manufactured by Popper).

Referring to FIG. 22, a sectional view of the endoscope 400 is shown. The sheath assembly 404 with the rod and lens assembly 412 and sterile barrier 410 is shown. The sterile barrier 410 and the rod and lens assembly 412 are attached to the mounting hub 414. The mounting hub 414 has a fiber optic window 420 which  
5 transmits light from a light source to a light sheath in an obturator. The window 420 can be a lens.

Still referring to FIG. 22, the rod and lens assembly 412 has a darkened outer tube 422 and a pair of object lenses 424. The distal end of the rod and lens assembly 412 will be discussed in further detail with reference to FIG. 27B.

10 Referring to FIG. 23, the base unit 402 of the endoscope 400 has a main scope body 428 with the CCD camera 430, a set of lenses 432, and a fiber optic tip mount 434 and fiber optic bundle 436 which define an opening 438 through which an optical image passes from the rod and lens assembly 412 towards the CCD camera 430. The opening 438 can be covered by a window or a lens. Still referring  
15 to FIG. 23, underlying the main scope body 428 is a fiber optic 442 which extends from the fiber optic light source connection 408 to fiber optic bundle 436.

FIG. 24 shows the rear portion of the base unit 402 of the endoscope 400. The electrical connection 406 is seen and in addition the fiber optic light source connection 408 is shown.

20 Referring to FIG. 25A, a front view of the base unit 402 is shown with the sheath assembly 404 removed. The base unit 402 has a plurality of fiber optic fibers 444 forming an annulus 445 surrounding the opening 438 as seen in FIG. 25B. The fiber optic bundle 436 is formed of these fiber optic fibers 444 in one embodiment. Alternately, the fiber optic bundle 436 has a single fiber optic fiber. The annulus  
25 445 can be a continuous circular pattern. Alternately, the annulus is formed of two semicircular portions 457. A slot 459 can separate the semicircular portions 457. The slot 459 can allow mechanical attachment of the light sheath 422, shown in Figure 27B to the hub 446.

Referring to FIG. 26, a side sectional view of the endoscope 400 is shown.  
30 The main scope body 428 as indicated above, has the CCD camera 430 which is connected through the electrical connection 406 to a monitor, such as illustrated in FIG. 1. The CCD camera 430 captures the image projected through the set of lenses

432 that is projected from the high index glass rod of the sheath assembly 404. While the sheath assembly is solid, the image that is projected through the lens 432 in the main scope body is through the opening 438. To light the image, the fiber optics 442 directs the light from the fiber optic light source connection 408 to the fibre optic bundle 436. The fiber optic bundle 436 can be formed of a plurality of fiber optics or from a single fiber optic.

Referring to FIG. 27A, the fiber optic bundle 436 projects its light through the lens 432 into the light sheath 448. The lens 432 can be a window, in an alternate embodiment. The connector between the bundle 436 and the lens 432 is shown in Figure 29A.

The disposable optic tube hub connector 446 with lens 432 can attach to an obturator or needle having a flushing port 450, as shown in Figure 26. The flushing port 450 can include a cap 452. The flushing port 450 allows a user the ability to flush a needle, after insertion into a surgical site, either when the rod and lens assembly 412 is located within the needle or has been removed from the needle. A fluid source, such as a syringe filled with saline, for example, can be attached to the port 450. When a user flushes the needle with saline while the rod and lens assembly 412 is located within the needle, the endoscope can block fluid from flowing from a proximal end of the needle, thereby concentrating flow through a distal end located within a surgical site. Alternately, for a user to flush the needle without the rod assembly 412 within the needle, the cap 452 can be used to cover the proximal end of the needle to direct the flow of the fluid to the distal end of the needle. Such flushing can allow clear viewing of a surgical site.

Referring to FIG. 27B, the distal end of the sheath assembly 404 has the light sheath 448 and encircles the disposable optic dark tube 422 containing the object lenses 424. Light can be transferred from the fiber optic bundle 436 through the light sheath and to an object being imaged.

FIG. 28 is a sectional view taken along the line 28-28 of FIG. 26. The figure shows a sectional view of the main scope body 428 cut through and looking up from the optical opening 438. The CCD 430 with connection 406 is shown. Likewise the lens 432 through which the image project are shown.

-22-

The fiber optic bundle 436, through which light is passed from the fiber optic 442, as shown in FIG. 26, encircles a portion of the optical opening 438 and directs light through the lens 432 in the disposable optics dark tube hub connector 446 into the light sheath surrounding the rod and lens assembly 412.

- 5        FIG. 29A is an enlarged sectional view of the interface of the fiber optic bundle 436, the disposable optics dark tube hub connector 446 and the mounting hub 414. While this invention has been particularly shown and described with references to preferred embodiments thereof, it will be understood by those skilled in the art that various changes in form and details may be made therein without
- 10    departing from the scope of the invention encompassed by the appended claims.



## CLAIMS

We claim:

1. A miniature endoscope comprising:
    - an optical waveguide that transmits an image, the waveguide having
    - 5 a diameter of less than 2 mm, and having a light absorbing layer;
    - an optical element coupled to a distal end of the waveguide;
    - an optical relay that is optically coupled to a proximal end of the waveguide; and
    - an imaging device mounted at a proximal end of the optical relay that
    - 10 receives an image from the optical waveguide.
  2. The miniature endoscope of Claim 1 wherein the endoscope has an outer diameter of 1.6 mm or less.
  3. The miniature endoscope of Claim 1 wherein the waveguide has an outer diameter between 0.6 and 1.6 mm.
  - 15 4. The miniature endoscope of Claim 1 wherein the endoscope further comprises an illumination channel and a binary phase ring which disperses light from the illumination channel.
  5. The miniature endoscope of Claim 1 wherein the waveguide comprises a glass having a refractive index in the range between 1.6 and 1.9.
  - 20 6. The miniature endoscope of Claim 1 wherein the waveguide comprises a glass rod.
- 
7. The miniature endoscope of Claim 1 wherein the light absorbing sheath comprises a thickness between 5 and 10  $\mu\text{m}$ .

-24-

8. The miniature endoscope of Claim 1 wherein the light absorbing sheath comprises extramural absorption glass.
9. The miniature endoscope of Claim 1 wherein the light absorbing sheath comprises a refractive index of 1.6 or less.
- 5 10. The miniature endoscope of Claim 1 wherein the illumination channel has a wall thickness in a range of 0.1 mm and 0.2 mm.
11. The miniature endoscope of Claim 1 wherein the illumination channel has a refractive index in a range between 1.4 and 1.6.
12. The miniature endoscope of Claim 1 wherein the illumination channel  
10 further comprises an outer sheath.
13. The miniature endoscope of Claim 12 wherein the outer sheath comprises a polyamide coating.
14. The miniature endoscope of Claim 13 wherein the polyamide coating has a thickness between 100 and 150  $\mu\text{m}$ .
- 15 15. The miniature endoscope of Claim 1 wherein the optical element comprises one or more lenses.
16. The miniature endoscope of Claim 1 wherein the optical element comprises a plastic lens.
17. The miniature endoscope of Claim 1 wherein the imaging device comprises a  
20 charge coupled device.
18. The miniature endoscope of Claim 1 wherein the endoscope further comprises a distal needle that penetrates tissue.

19. The miniature endoscope of Claim 1 wherein the optical element has a rectangular cross-sectional area.
  20. The miniature endoscope of Claim 1 wherein the waveguide has a rectangular cross-sectional area.
  - 5 21. The miniature endoscope of Claim 1 wherein the optical relay has a rectangular cross-sectional area.
  22. The miniature endoscope of Claim 1 further comprising a handle in which the optical relay and imaging device are positioned.
  23. The miniature endoscope of Claim 22 further comprising an illumination  
10 channel that is optically coupled to a light source in the handle.
  24. The miniature endoscope of Claim 22 further comprising a coupler that connects the handle to the optical waveguide.
  25. The miniature endoscope of Claim 22 further comprising a disposable sheath that extends over the handle.
  - 15 26. The miniature endoscope of Claim 25 wherein the sheath is attached to a rigid waveguide housing that is connected to the handle.
  27. The miniature endoscope of Claim 1 further comprising a light source that is optically coupled to the optical waveguide.
- 
28. A miniature endoscope comprising:  
20 an imaging channel having a diameter less than 2 mm, and a light absorbing layer defining a channel boundary;

-26-

an illumination channel having a first layer on an inner surface of the illumination channel and a second layer on an outer surface of the illumination channel;

an optical element coupled to a distal end of the imaging channel;

5 an optical relay coupled to a proximal end of the imaging channel;

and

an imaging device coupled to a proximal end of the optical relay.

29. The miniature endoscope of Claim 28 wherein the imaging device comprises a charge coupled device.
- 10 30. The miniature endoscope of Claim 28 wherein the imaging channel comprises a transparent material having a refractive index of at least 1.6.
31. The miniature endoscope of Claim 30 wherein the imaging light channel comprises a glass rod.
- 15 32. The miniature endoscope of Claim 31 wherein the glass rod comprises an F2 or an F7 glass.
33. The miniature endoscope of Claim 28 wherein the light absorbing layer comprises a light absorbing glass.
34. The miniature endoscope of Claim 33 wherein the light absorbing layer comprises a B6-2 glass or a BG-4 glass.
- 20 35. The miniature endoscope of Claim 28 wherein the illumination channel is coupled to a light source.
36. The miniature endoscope of Claim 28 wherein the illumination channel comprises a material having a refractive index higher than the first layer and the second layer.

-27-

37. The miniature endoscope of Claim 28 wherein the illumination channel comprises a transparent material having a refractive index of at least 1.6.
38. The miniature endoscope of Claim 28 wherein the first layer and the second layer each have index of refraction of less than 1.6.
- 5 39. The miniature endoscope of Claim 28 wherein the endoscope has a handle and a rigid channel having connected to the handle with a coupler.
40. The miniature endoscope of Claim 28 wherein the optical element has a rectangular cross-sectional area.
41. The miniature endoscope of Claim 28 wherein the imaging channel has a  
10 rectangular cross-sectional area.
42. The miniature endoscope of Claim 28 wherein the optical relay has a rectangular cross-sectional area.
43. A method of forming a reflective boundary on a glass channel for a microendoscope comprising the steps:  
15       providing a glass channel for a microendoscope;  
          providing a light absorbing material;  
          extruding the light absorbing material over the glass channel to form a reflective boundary on the glass channel.
44. The method of Claim 43 further comprising the step of using a fiber optic  
20 ~~drawing process to extrude the light absorbing material over the glass~~  
channel.

45. The method of Claim 43 further comprising the step of using a bar-in-tube drawing process to extrude the light absorbing material over the glass channel.
46. A method of forming an image light channel for a microendoscope comprising the steps:
- 5                   providing an illumination channel having a refractive index;  
                  coating an inner surface and an outer surface of the illumination channel with a material having a refractive index lower than the illumination channel refractive index;
- 10                  providing an image light channel for a microendoscope; and  
                  attaching the illumination channel to the image light channel.
47. The method of Claim 46 further comprising the step of using a tube-extrusion process for form the coatings on the illumination channel.
48. The method of Claim 46 further comprising the step of depositing a glass on
- 15                  the outer surface and the inner surface of the illumination channel.
49. The method of Claim 46 further comprising the step of using a bar-in-tube fiber drawing process to fuse the illumination channel to the image light channel.
50. A method of forming a cladding structure on an image light channel for a
- 20                  microendoscope comprising the steps:
- providing an image light channel;  
                  forming a material having an index of refraction on the image light channel that is lower than the index of refraction of the image light channel to form a first cladding;
- 25                  extruding an illumination channel over the first cladding on the image light channel; and  
                  forming a second cladding on the illumination channel.

51. A miniature endoscope comprising:  
a handle having an imaging device, a light source and a first coupling element;  
a rigid probe having a waveguide and a second coupling element that  
5 connects the probe to the first coupling element, the waveguide having a light absorbing boundary.
52. The endoscope of Claim 51 further comprising:  
a beamsplitter mounted within the housing wherein the beamsplitter directs light from the lighting source through a rod and lens assembly to an  
10 object such that the beamsplitter receives light from an object through the rod and lens assembly and directs the light to the imaging device.
53. The endoscope of Claim 51 wherein the waveguide comprises a hollow channel.
54. The miniature endoscope of Claim 51 wherein the imaging device comprises  
15 a plurality of lenses and a polarizer.
55. The miniature endoscope of Claim 54 wherein the polarizer comprises a sheet polarizer.
56. The miniature endoscope of Claim 54 wherein the polarizer comprises a cross polarizer.
- 20 57. The miniature endoscope of Claim 56 wherein the cross polarizer comprises a first prism and a second prism.
- 
58. The miniature endoscope of Claim 51 wherein the light source is coupled to a polarizer and a lens.

-30-

59. The miniature endoscope of Claim 51 wherein the light source is coupled to an illumination channel with a fiber optic element.
60. The miniature endoscope of Claim 51 wherein the probe comprises an annular illumination channel around the waveguide.
- 5 61. The miniature endoscope of Claim 51 wherein the light source comprises an external lamp.
62. The miniature endoscope of Claim 61 wherein the external lamp comprises a xenon light source.
63. The miniature endoscope of Claim 51 wherein the endoscope further  
10 comprises a sheath attached to the probe and extending over the handle.
64. The miniature endoscope of Claim 53 wherein the sheath comprises a sterile barrier .
65. The miniature endoscope of Claim 51 wherein the probe comprises a needle with a distal optical system.
- 15 66. The miniature endoscope of Claim 51 further comprising a cannula wherein the probe fits within the cannula.
67. The miniature endoscope of Claim 51 wherein waveguide comprises a rod and lens assembly having a locking mechanism wherein the cannula locks onto the rod and lens assembly.
- 20 68. The miniature endoscope of Claim 66 wherein the cannula comprises an illumination channel.



69. The miniature endoscope of Claim 66 wherein the cannula further comprises a stylet.
70. A method of using a miniature endoscope comprising:  
providing a base unit and a sheath assembly having a probe  
5 waveguide and a sterile barrier; and  
attaching the sheath assembly to the base unit such that the sterile  
barrier extends over the base unit.
71. The method of Claim 70 further comprising providing a cannula and  
securing the cannula to the sheath assembly.
- 10 72. The method of Claim 70 further comprising providing a luer fitting on the  
sheath assembly.
73. The method of Claim 70 further comprising disposing of the sheath assembly  
after use and attaching a second sheath assembly to the base unit for further  
use.
- 15 74. The method of Claim 70 further comprising providing a probe waveguide  
having a hollow channel and a light absorbing channel wall.
75. The method of Claim 70 further comprising providing a base unit including a  
handle, an imaging device within the handle and a relay optical system that  
couples an image from the waveguide to the imaging device.
- 20 76. The method of Claim 70 further comprising providing a probe waveguide  
having a diameter of 2 mm or less.
- 
77. The method of Claim 70 further comprising connecting the base unit to a  
display.

-32-

78. The method of Claim 70 further comprising providing an annular illumination channel in the probe.
79. The method of Claim 70 further comprising providing a probe waveguide having a length between 2 cm and 10 cm.
- 5 80. The method of Claim 70 further comprising directing polarized light through the waveguide.

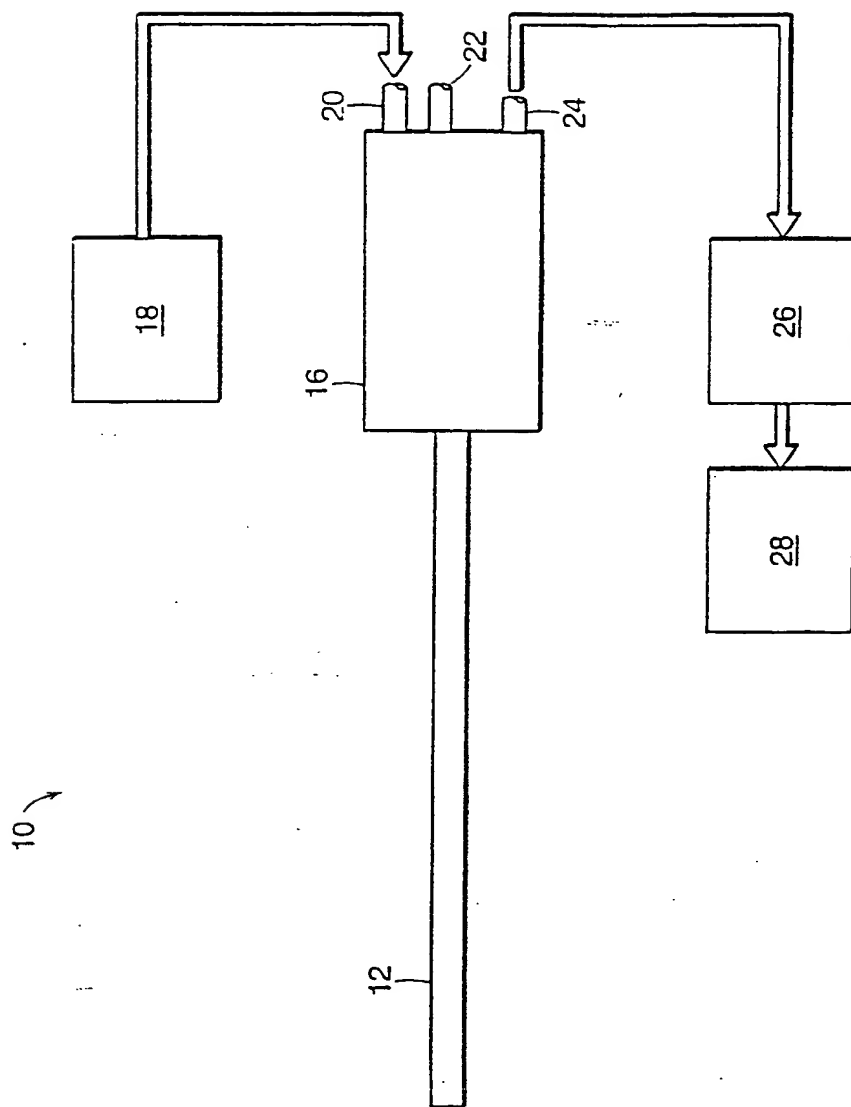


FIG. 1

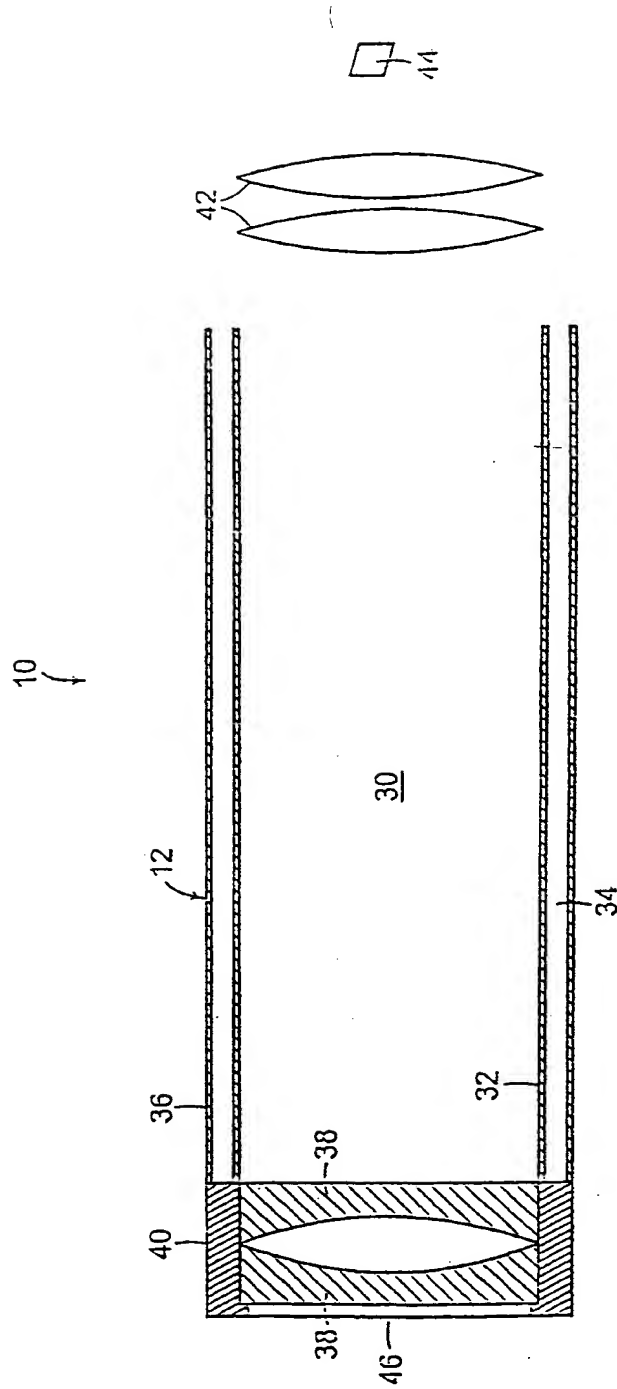


FIG. 2

3/20

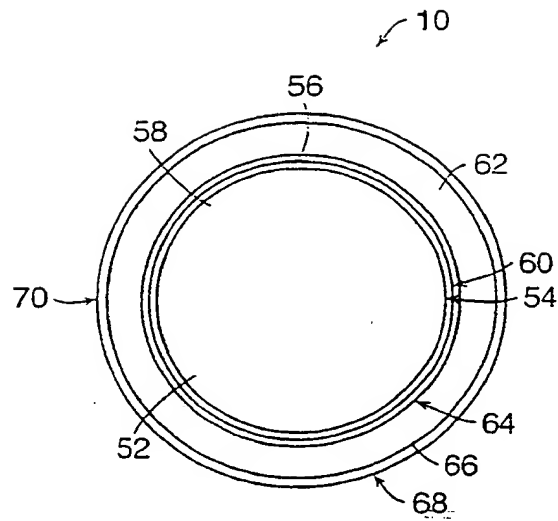


FIG. 3

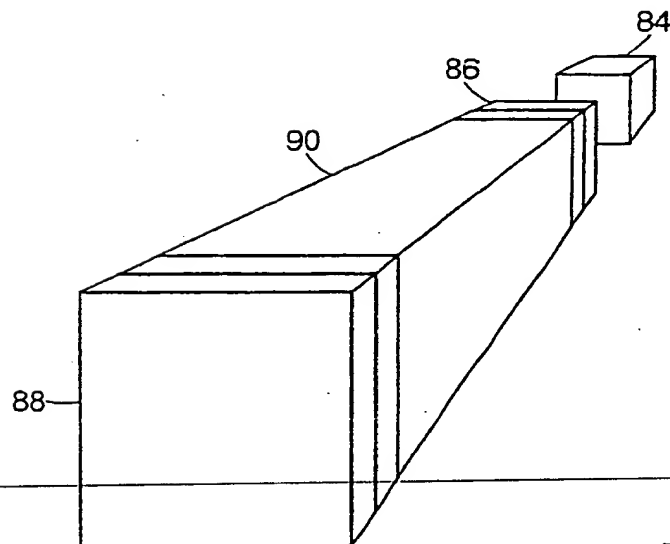


FIG. 5

4/20

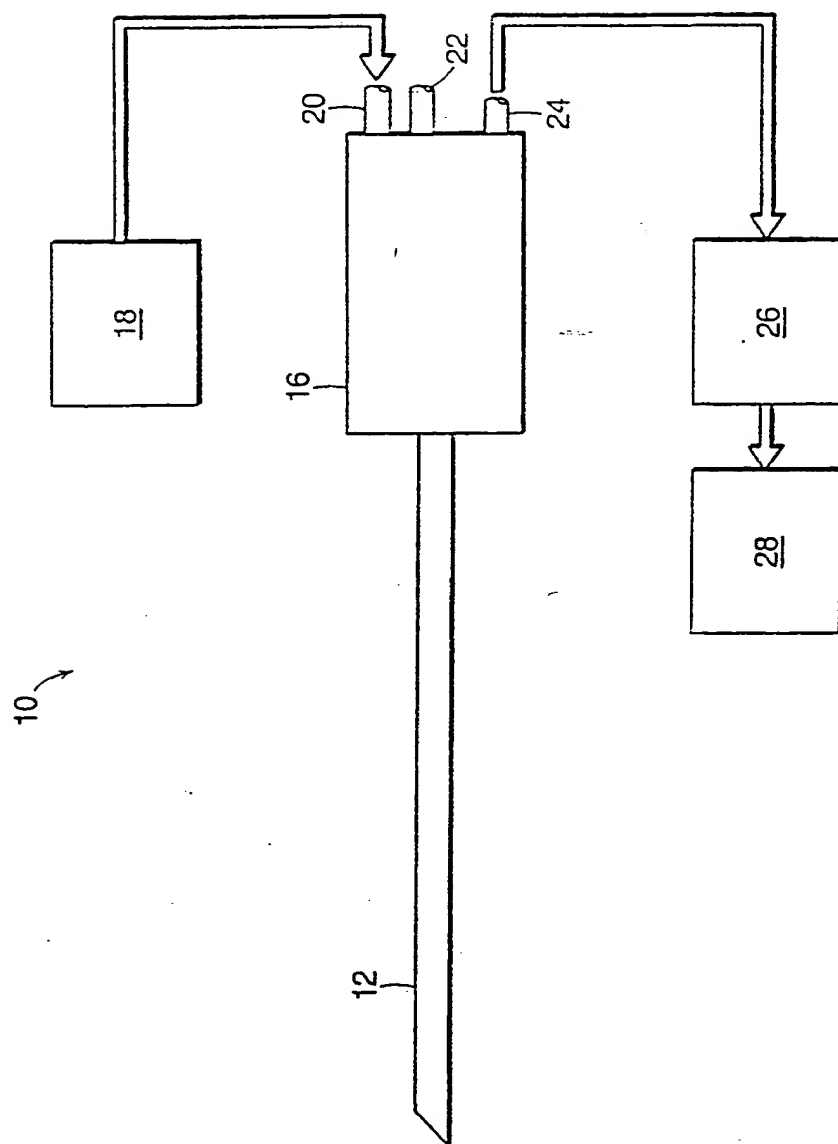


FIG. 4

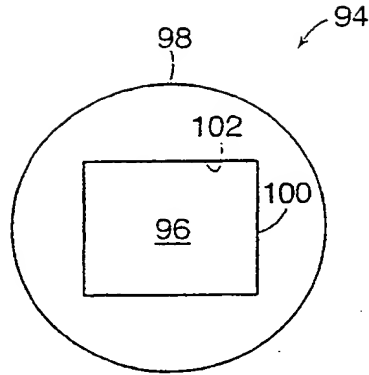


FIG. 6

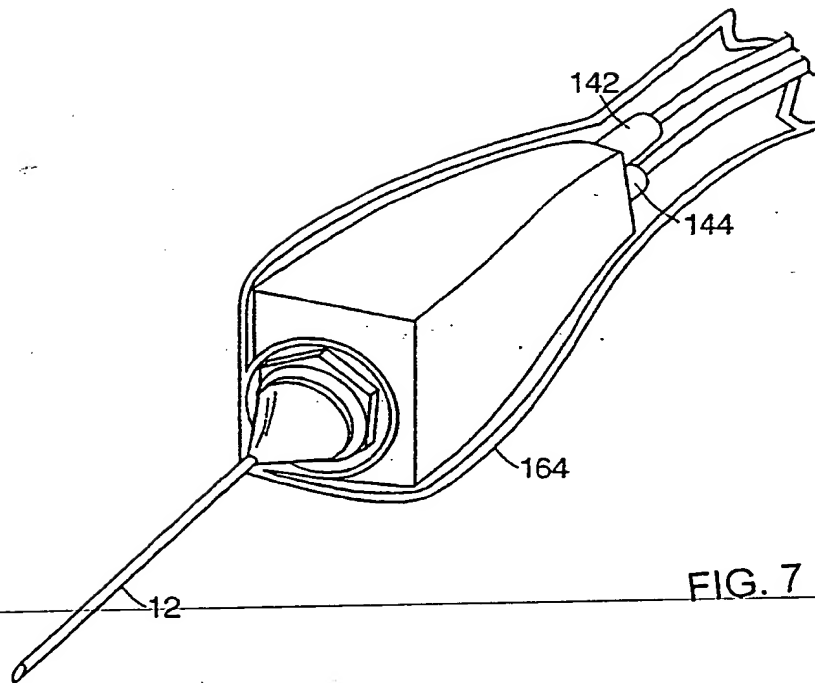


FIG. 7

6/20

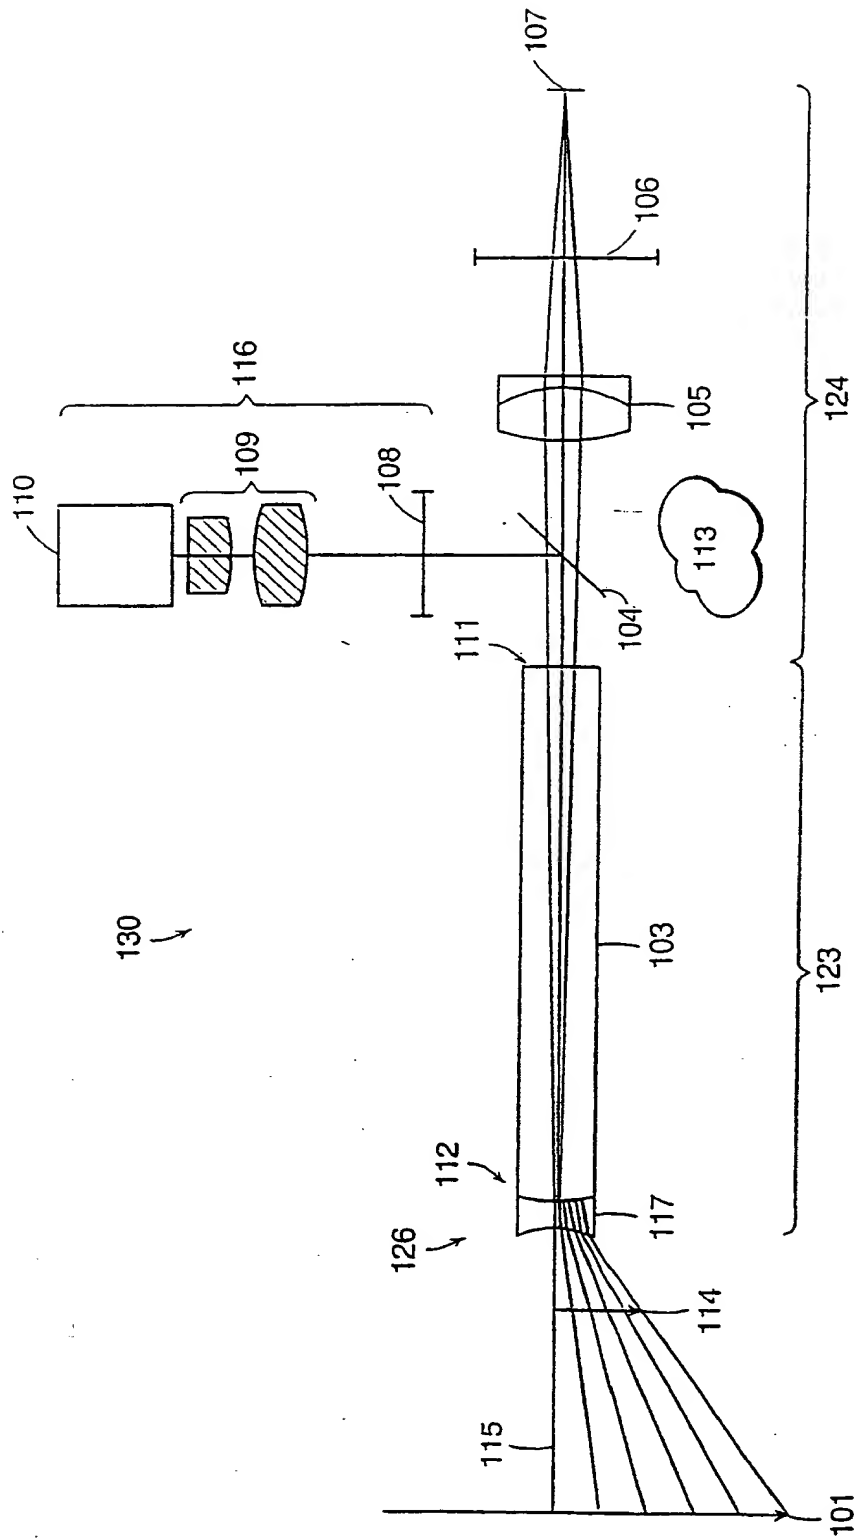


FIG. 8



7/20

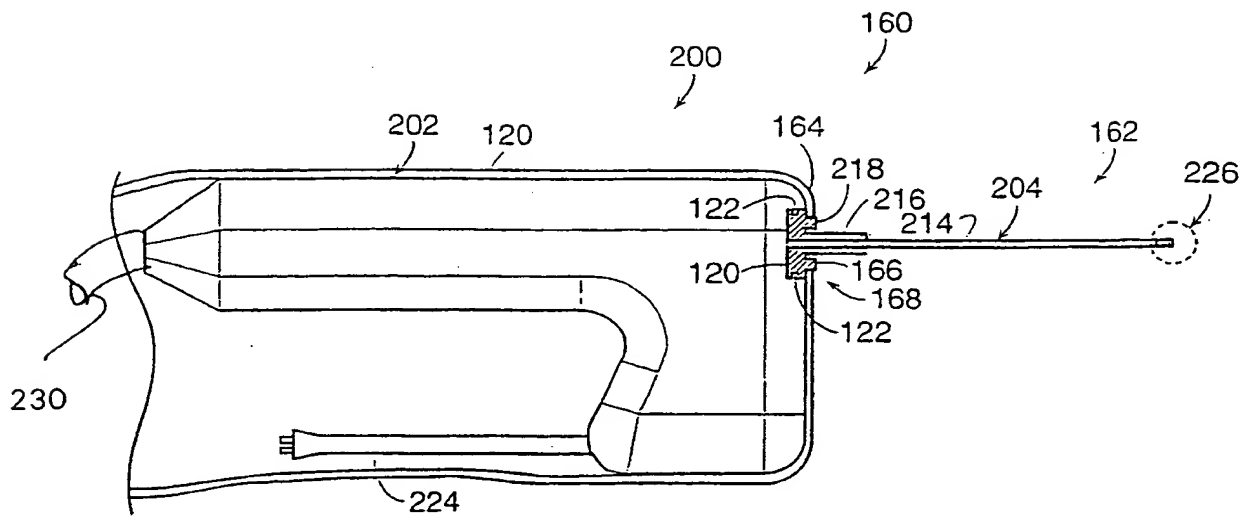


FIG. 9

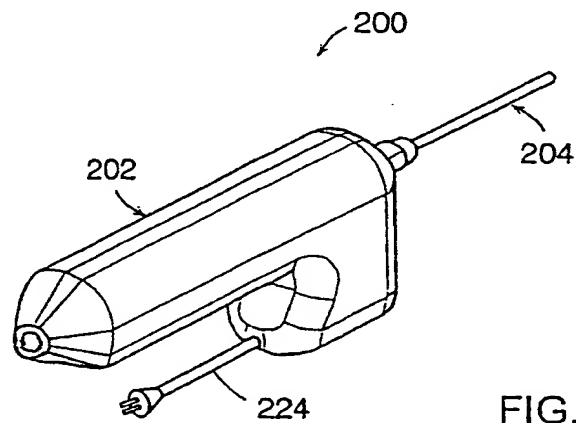


FIG. 10

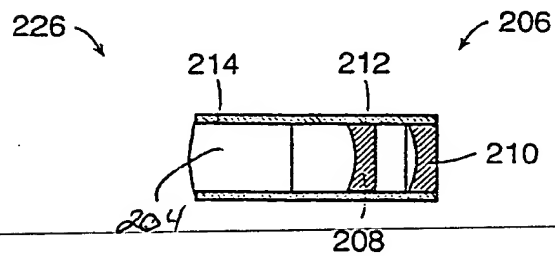


FIG. 11

8/20

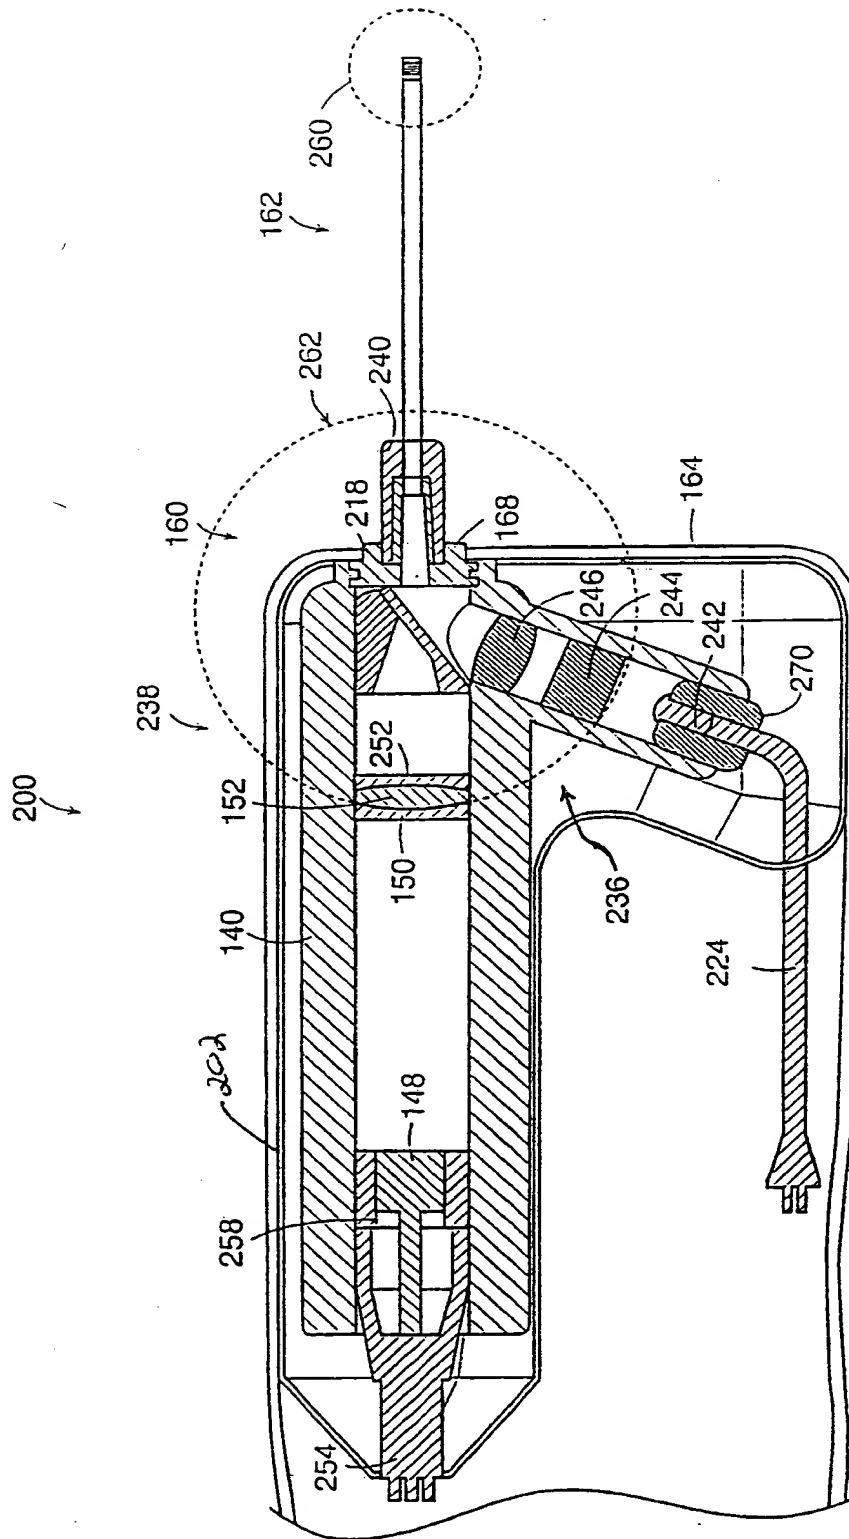
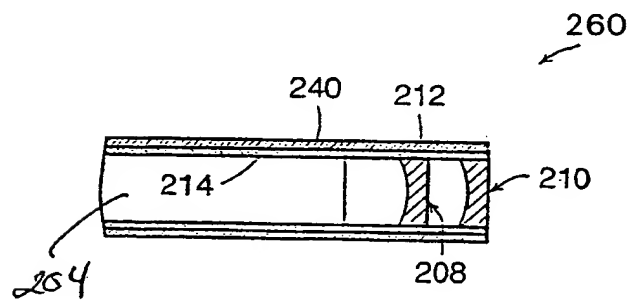
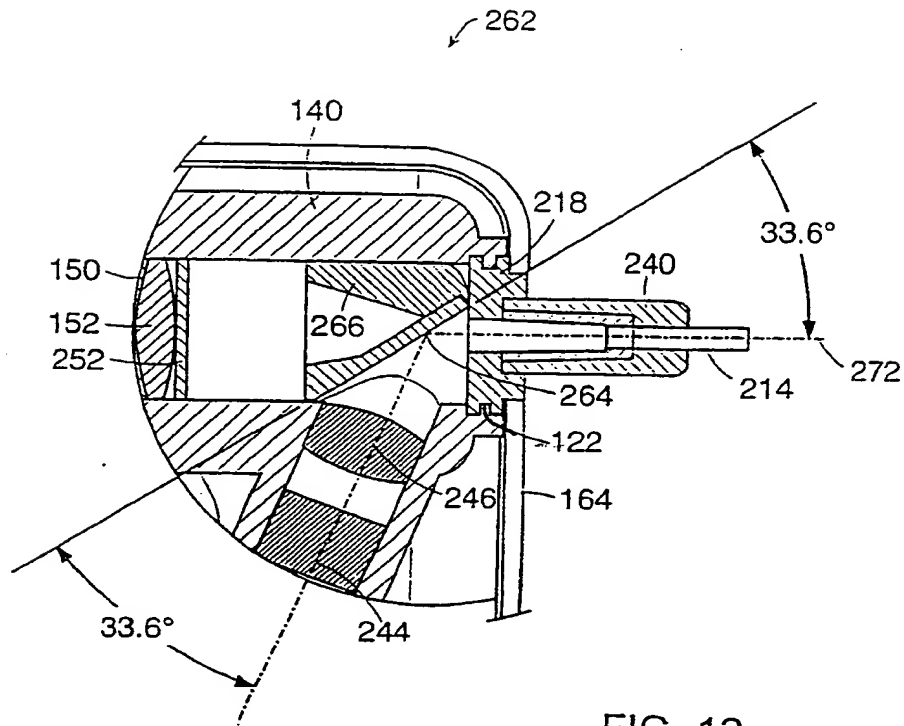


FIG. 12

**SUBSTITUTE SHEET (RULE 26)**



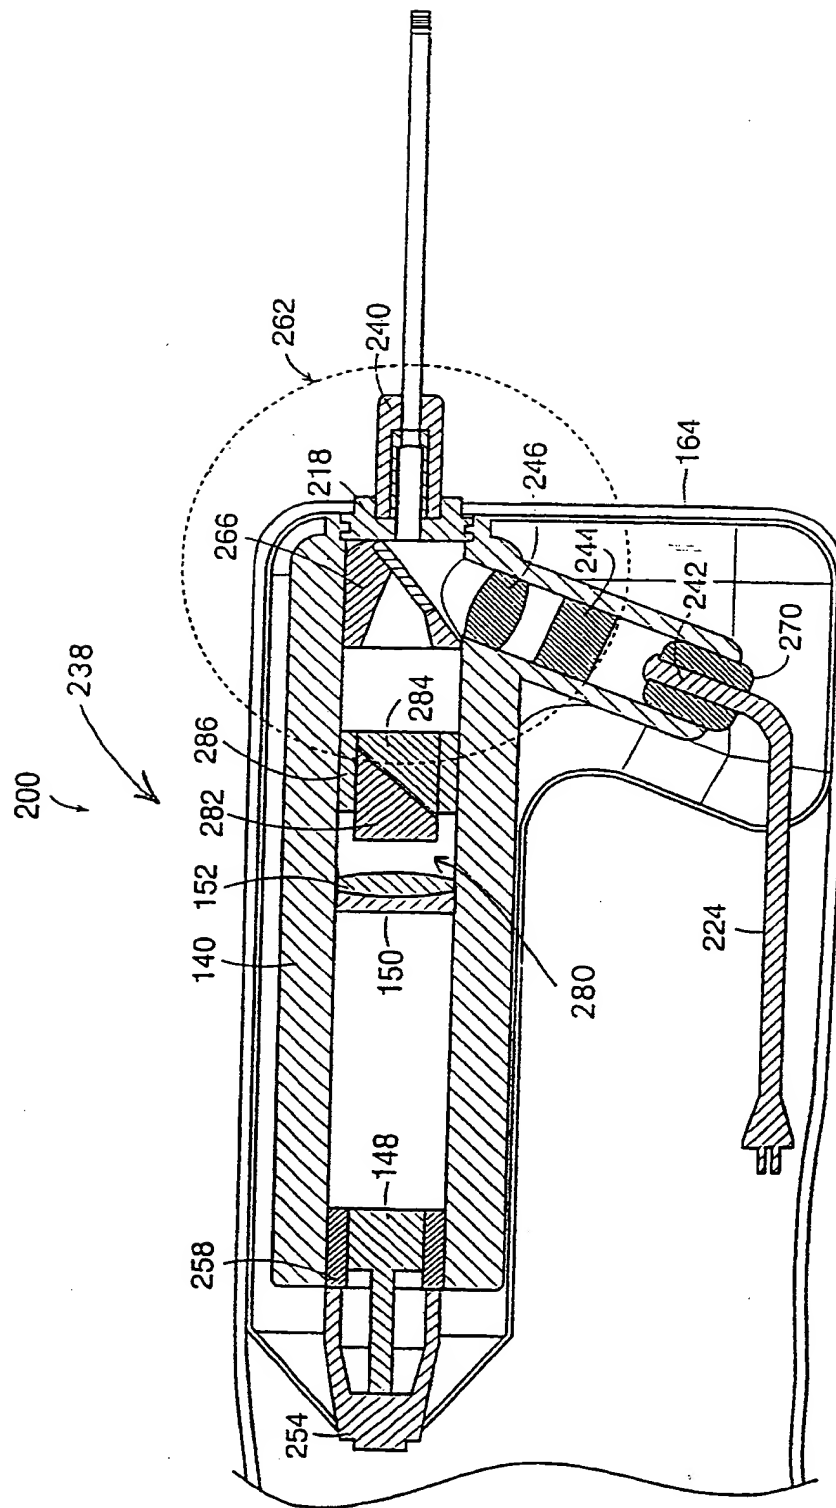


FIG. 15

**SUBSTITUTE SHEET (RULE 26)**

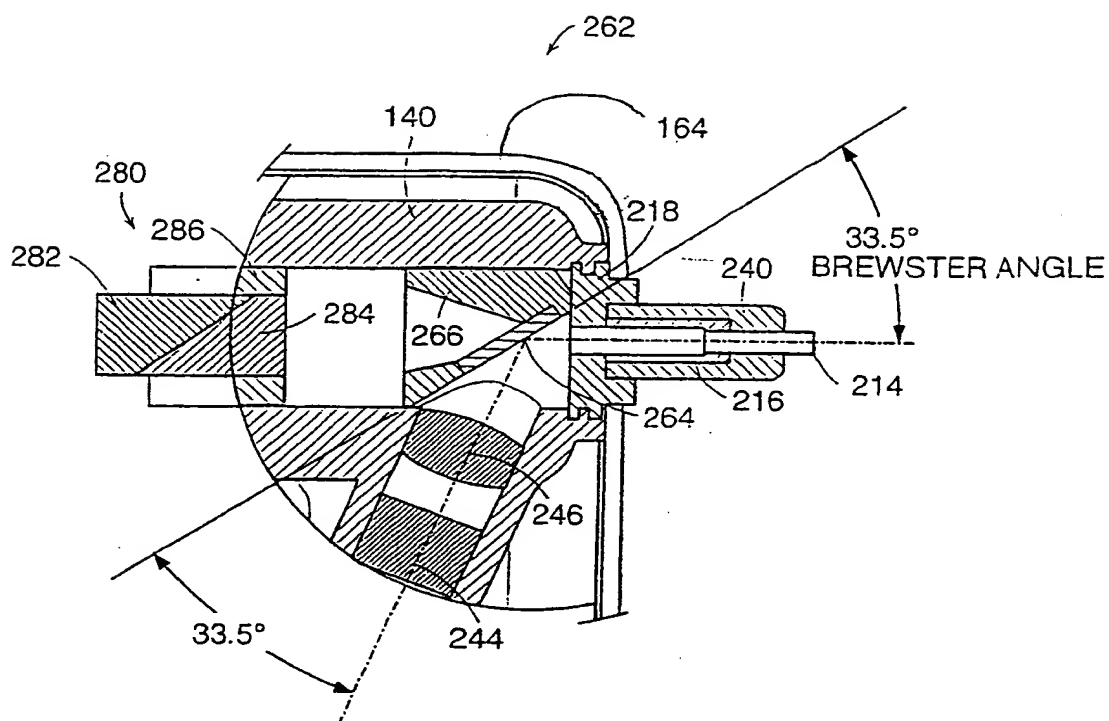


FIG. 16

**SUBSTITUTE SHEET (RULE 26)**

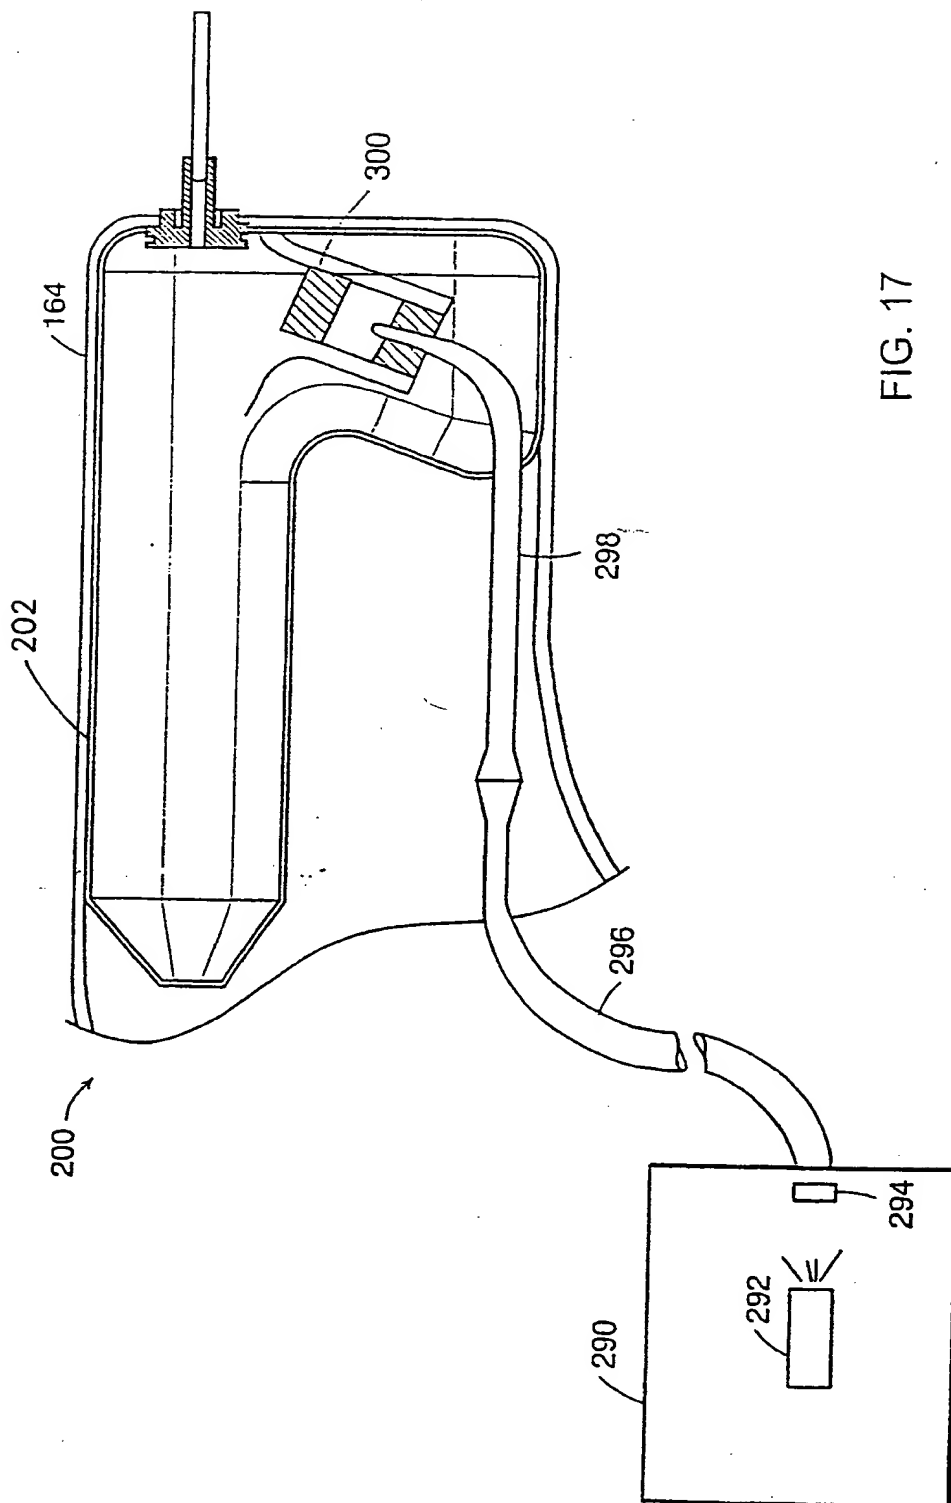


FIG. 17

13/20

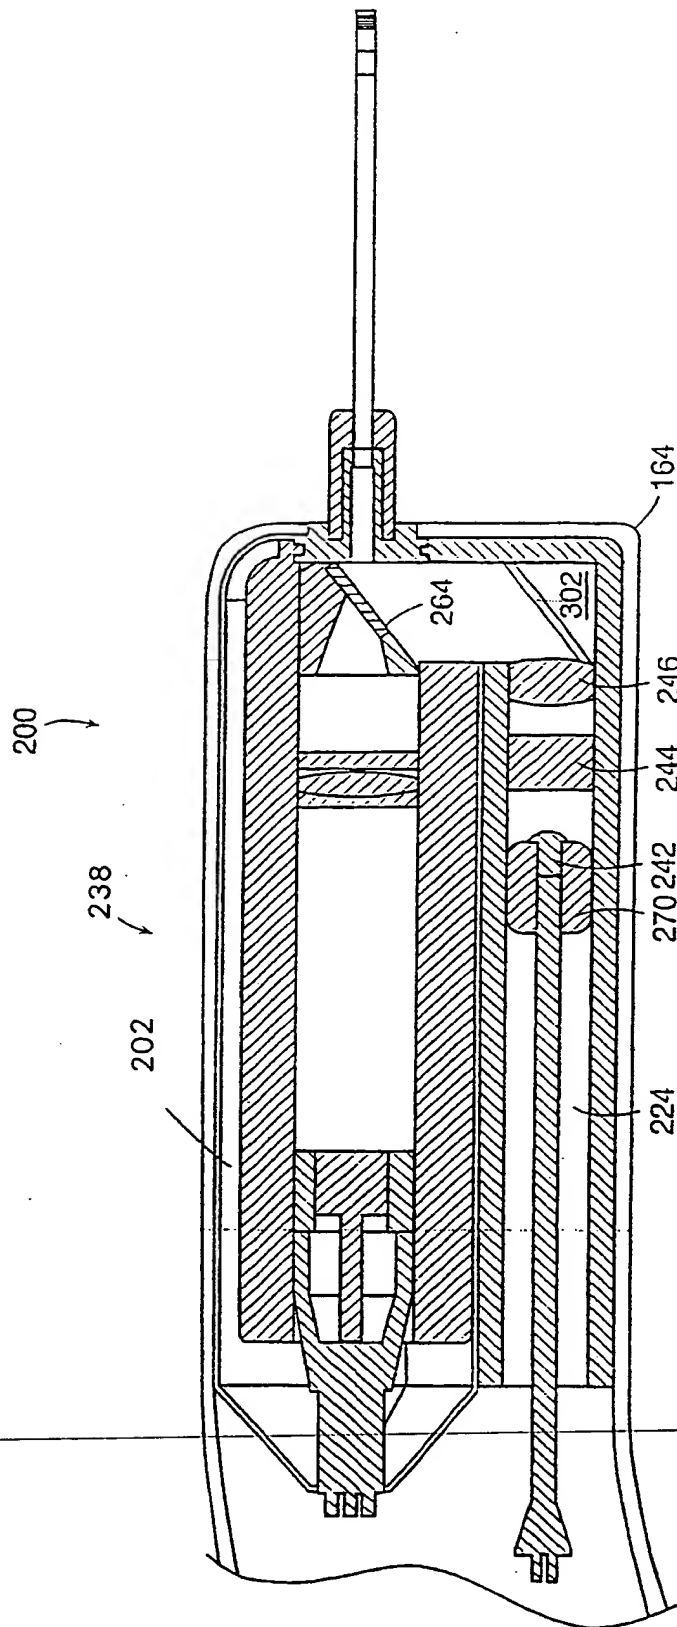


FIG. 18

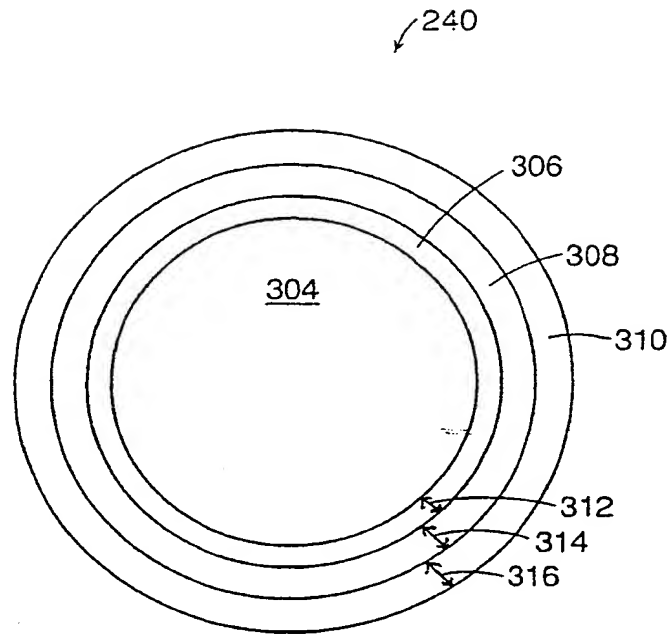


FIG. 19


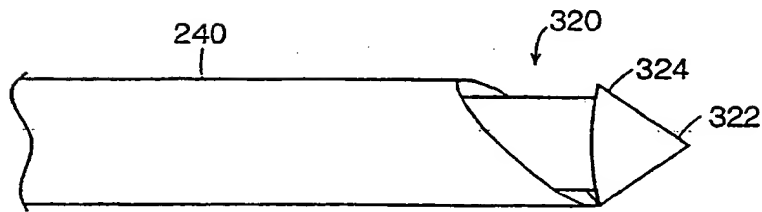


FIG. 20



15/20

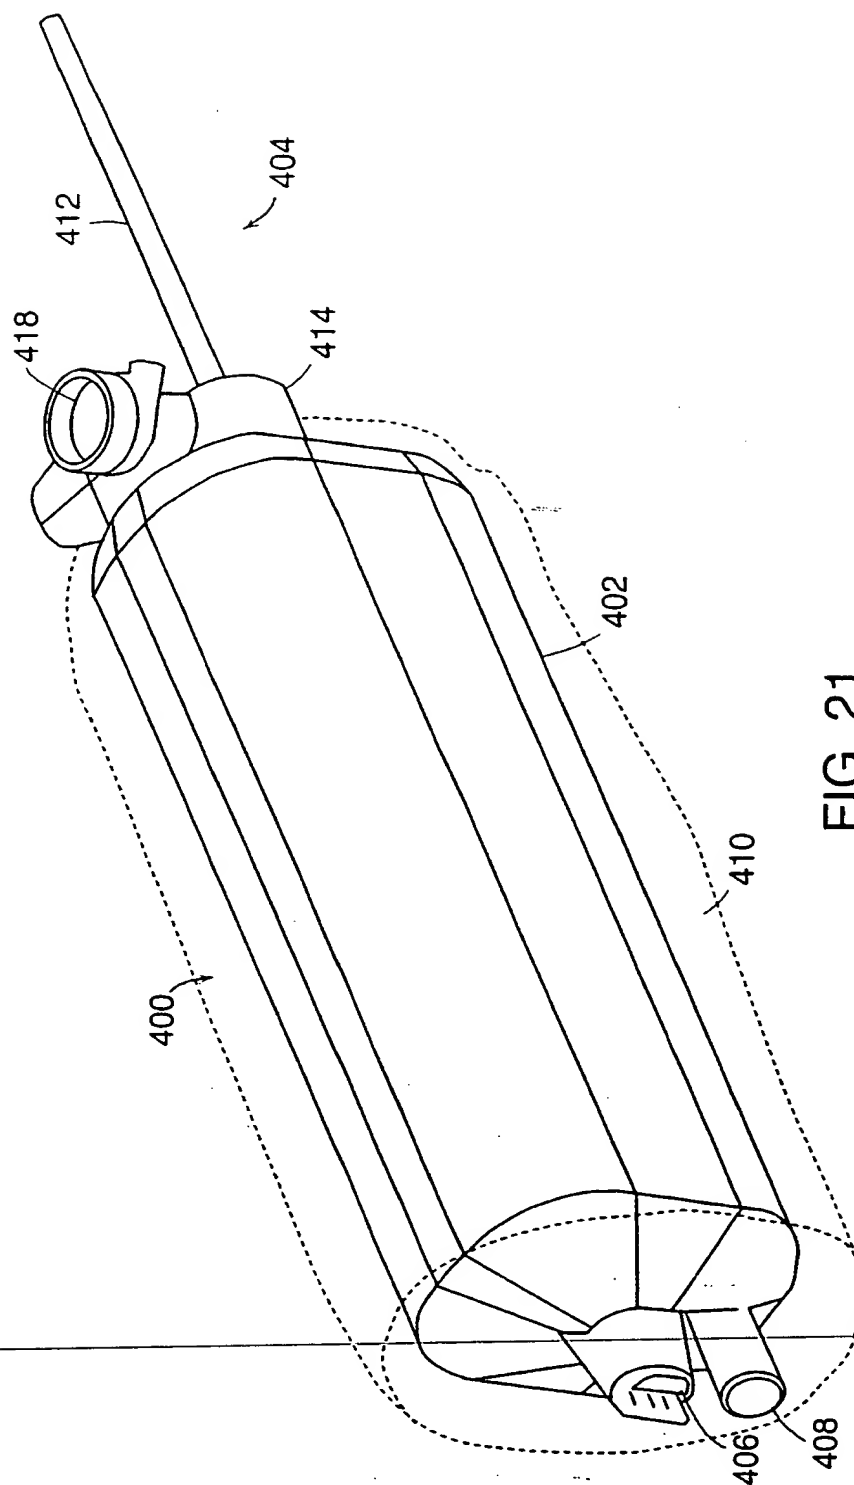

SUBSTITUTE SHEET (RULE 26)

16/20

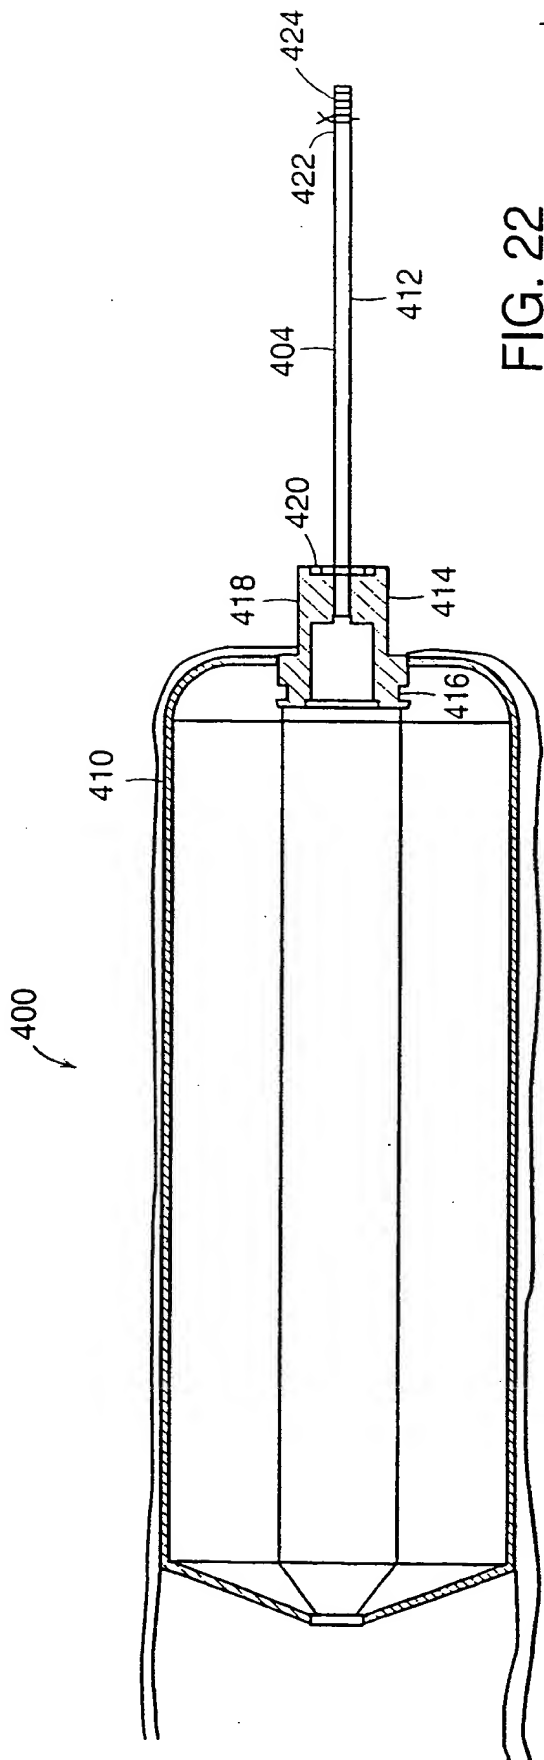


FIG. 22

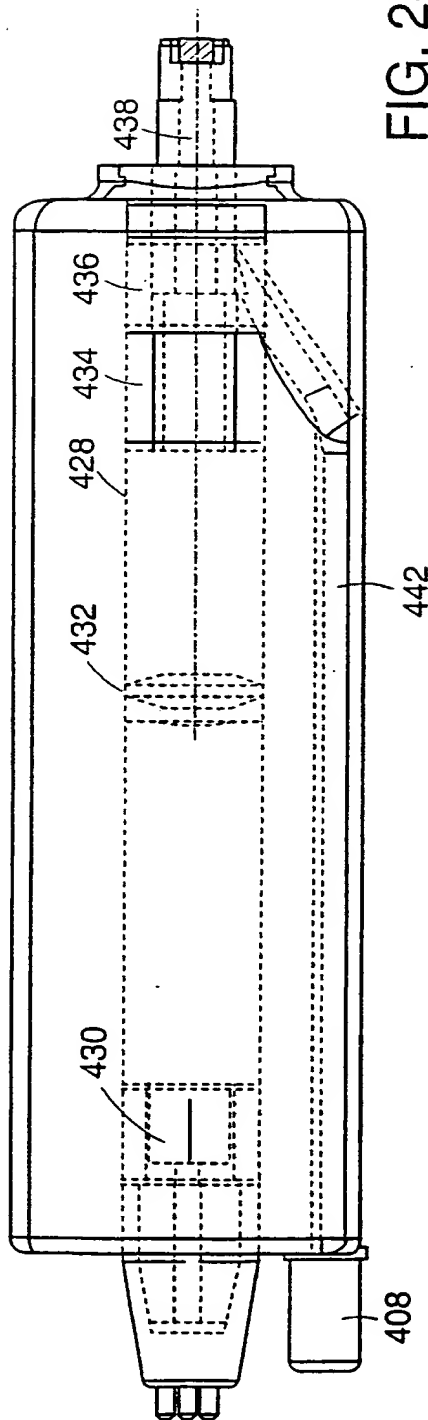


FIG. 23

SUBSTITUTE SHEET (RULE 26)

17/20

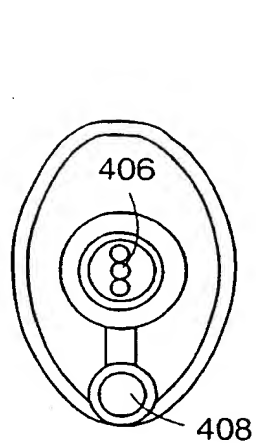


FIG. 24

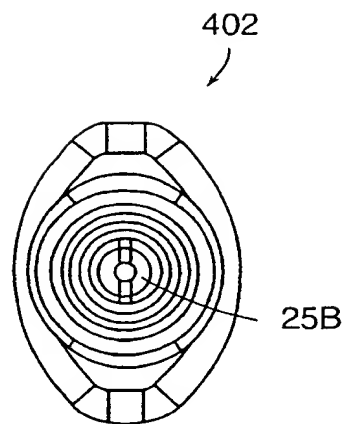


FIG. 25A

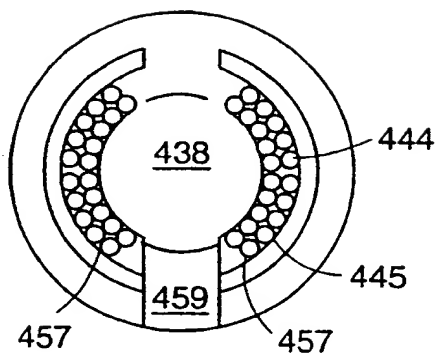


FIG. 25B

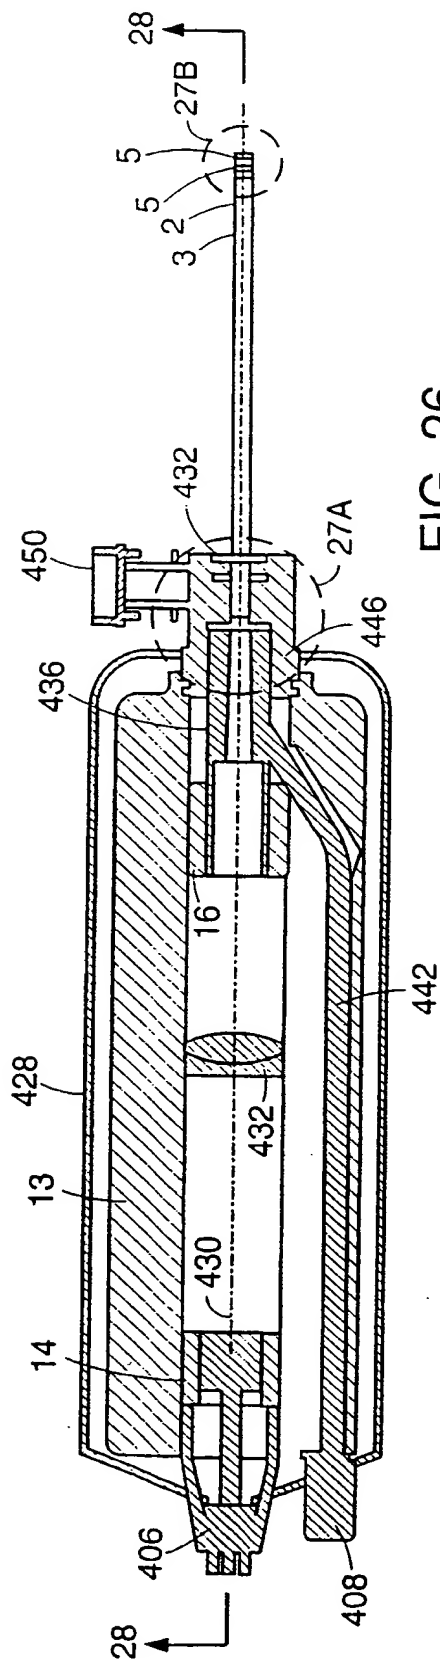


FIG. 26

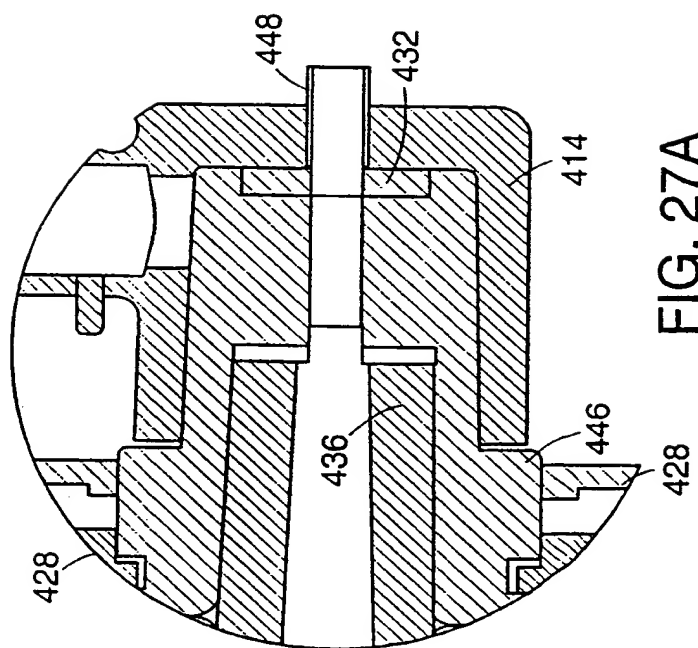


FIG. 27A




FIG. 27B

19/20

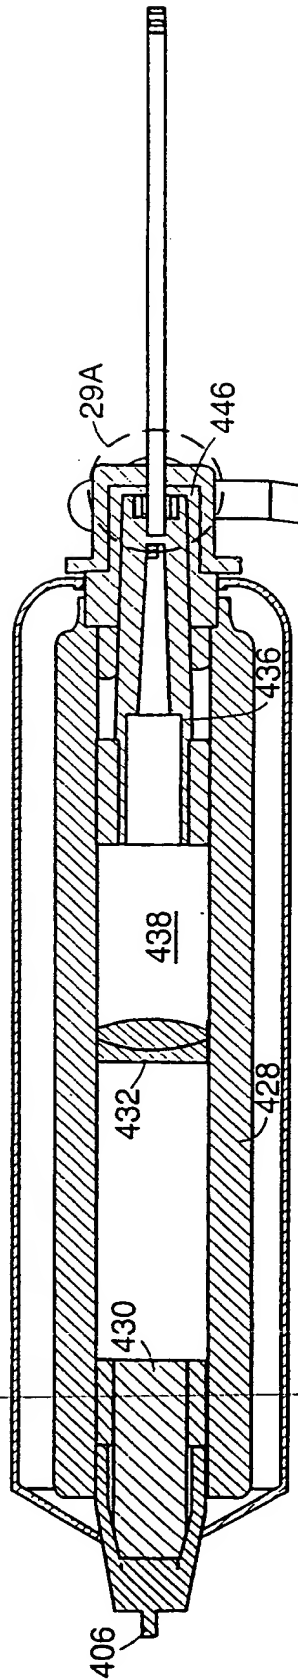


FIG. 28

20/20


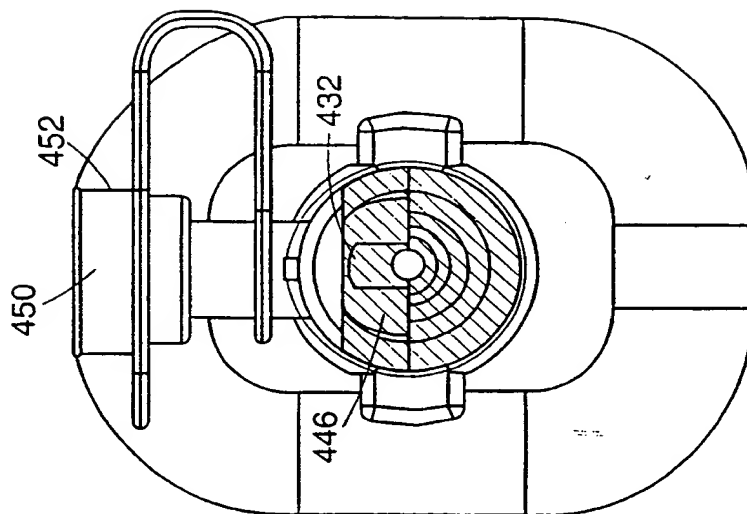


FIG. 29B

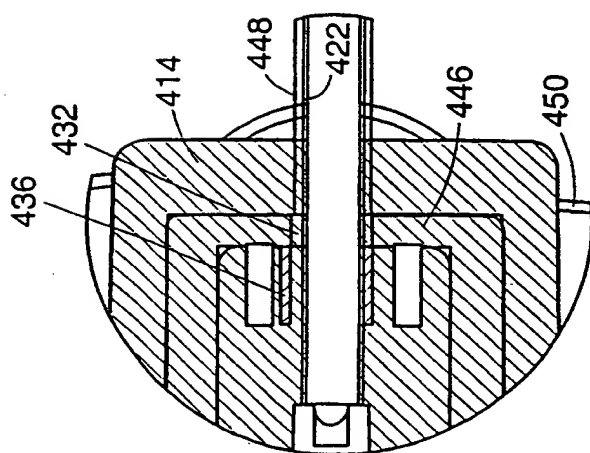

FIBER OPTIC CONNECTION TRANSMITS  
LIGHT TO LIGHT-SHEATH THROUGH OPTICS HUB  
WINDOW/LENS IN DISPOSABLE OPTICS TIP ASSEMBLY

FIG. 29A

## INTERNATIONAL SEARCH REPORT

Int ional Application No

PCT/US 00/25107

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61B1/04 A61B1/313 A61B1/002

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B G02B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, PAJ, WPI Data

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X          A	EP 0 316 244 A (WELCH ALLYN INC) 17 May 1989 (1989-05-17)   column 2, line 11 - line 60   column 3, line 12 -column 5, line 9; tables 1-3  ---  -/--	1-3,6, 15,17, 22,23, 28,29, 31, 59-61, 76-78 5,8,27, 35,36, 46,51,53



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

## \* Special categories of cited documents:

- \*A\* document defining the general state of the art which is not considered to be of particular relevance
- \*E\* earlier document but published on or after the international filing date
- \*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- \*O\* document referring to an oral disclosure, use, exhibition or other means
- \*P\* document published prior to the international filing date but later than the priority date claimed

- \*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- \*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- \*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- \*Z\* document member of the same patent family

Date of the actual completion of the international search

15 January 2001

Date of mailing of the international search report

23/01/2001

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Weihs, J

## INTERNATIONAL SEARCH REPORT

Int ional Application No

PCT/US 00/25107

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	ROL P ET AL: "OPTICAL PROPERTIES OF MINIATURIZED ENDOSCOPES FOR OPHTHALMIC USE" OPTICAL ENGINEERING, US, SOC. OF PHOTO-OPTICAL INSTRUMENTATION ENGINEERS. BELLINGHAM, vol. 34, no. 7, 1 July 1995 (1995-07-01), pages 2070-2076, XP000517073 ISSN: 0091-3286	1-3, 6, 12, 15, 17, 22, 29, 31, 76, 77
A	page 2071, left-hand column, line 3 -page 2076, left-hand column, line 30; tables 1-9	5, 8, 23, 28, 30
A	WO 94 14367 A (SCHOTT FIBER OPTICS INC ; SIEGMUND WALTER P (US); REMIJAN PAUL W (U) 7 July 1994 (1994-07-07)	1, 4-6, 8, 12, 15, 17, 19-24, 27-31, 33, 35, 39-46, 48, 49, 51, 53, 54, 59-62, 64, 67, 68, 70, 74, 75, 77
A	page 7, line 5 -page 14, line 25; tables 1-9  US 5 630 784 A (SIEGMUND WALTER P ET AL) 20 May 1997 (1997-05-20)	1, 4-6, 8, 12, 15, 17, 19-24, 27-31, 33, 35, 39-46, 48, 49, 51, 53, 54, 59, 60, 64, 67, 68, 74, 75, 77, 78
	column 3, line 39 -column 6, line 24; tables 1-9	

Form PCT/ISA/210 (continuation of second sheet) (July 1992)



## INTERNATIONAL SEARCH REPORT

Information on patent family members

Int ional Application No

PCT/US 00/25107

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP 0316244 A	17-05-1989	US 4854302 A	08-08-1989
		DE 3868233 A	12-03-1992
		JP 1155826 A	19-06-1989
WO 9414367 A	07-07-1994	US 5423312 A	13-06-1995
		AU 5985494 A	19-07-1994
		EP 0673220 A	27-09-1995
		JP 8507871 T	20-08-1996
		US 5630784 A	20-05-1997
US 5630784 A	20-05-1997	US 5423312 A	13-06-1995
		AU 5985494 A	19-07-1994
		EP 0673220 A	27-09-1995
		JP 8507871 T	20-08-1996
		WO 9414367 A	07-07-1994

**This Page Blank (uspto)**

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image  
problems checked, please do not report these problems to  
the IFW Image Problem Mailbox.**

**BEST AVAILABLE COPY**